


# BeneVision TM80

## Telemetry Monitor

1. Turn on the device

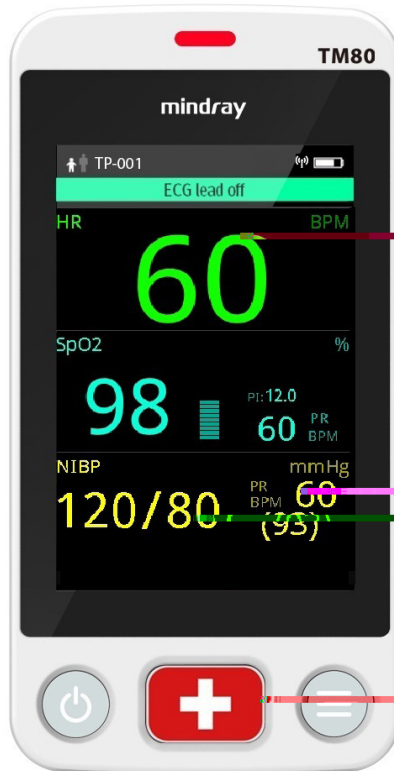

**mindray**

**Note:** The  $L^p$  norm is defined as  $\|f\|_p = \left( \int |f|^p \right)^{1/p}$ . For  $p=1$ , this is the total area under the curve. For  $p=2$ , it is the square root of the area under the curve squared. For  $p=\infty$ , it is the maximum value of the function.

# Table of Contents

---


<b>TM80 Physical View</b> .....	<b>1</b>
<b>General Navigation</b> .....	<b>3</b>
▶ Home	3
▶ Back	3
▶ Home, Back, and Lockscreen	3
<b>Patient Setup</b> .....	<b>6</b>
▶ Add	6
▶ Manage	6
▶ Edit Existing Patient	6
<b>Standby</b> .....	<b>7</b>
▶ Standby	7
▶ Standby Locking	7
<b>Printing</b> .....	<b>8</b>
<b>Nurse Call</b> .....	<b>8</b>
▶ Nurse Call	8
▶ Nurse Call Response	8
<b>ECG</b> .....	<b>9</b>
▶ ECG	9
▶ ECG Lock	9
▶ ECG Print	9
<b>Resp</b> .....	<b>11</b>
▶ Resp	11
<b>SpO<sub>2</sub> (OPTIONAL)</b> .....	<b>12</b>
▶ SpO <sub>2</sub> Lock	12
▶ SpO <sub>2</sub> Lockscreen	12
<b>NIBP (OPTIONAL)</b> .....	<b>14</b>

## Table of Contents (cont'd)

---

• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
<b>Technical Alarms</b> .....	<b>15</b>
• <b>Auto Lock</b> ▼	15
<b>Screen Display</b> .....	<b>16</b>
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
<b>Screen Lock/View Only Mode</b> .....	<b>17</b>
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
<b>Adjust Volumes</b> .....	<b>18</b>
<b>Parameter Colors</b> .....	<b>19</b>
<b>Clean/Disinfect the TM80</b> .....	<b>19</b>
• <b>Auto Lock</b> ▼	15
• <b>Auto Lock</b> ▼	15
<b>Clean/Disinfect Reusable Accessories</b> .....	<b>23</b>
<b>Sterilization</b> .....	<b>23</b>

## TM80 PHYSICAL VIEW

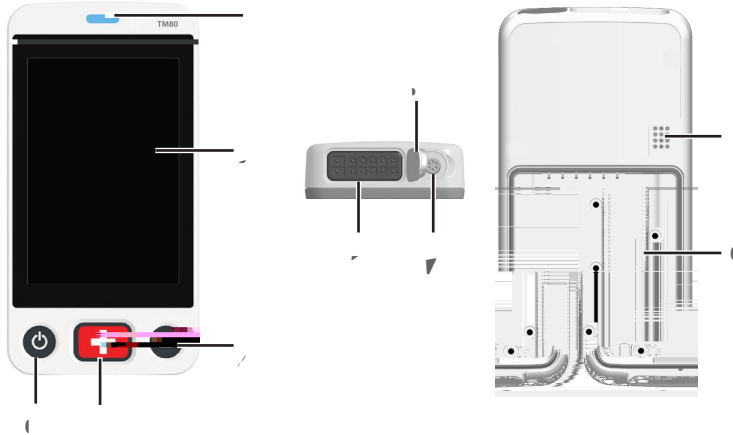

### 1. Front View (Physical)

1.1. Screen (L)

- Screen resolution: 1280 x 800

1.2. Power Button (L)

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

- Power button: Physical button on the left side of the device.

## QUESTION

1. The following are the components of a company's operating cycle:

(a) Payables

(b) Inventory

(c) Receivables

(d) Cash

2. The following are the components of a company's operating cycle:

(a) Payables

(b) Inventory





(c) Cash

(d) Receivables

3. The following are the components of a company's operating cycle:

## GENERAL NAVIGATION

### Swipe for More Data

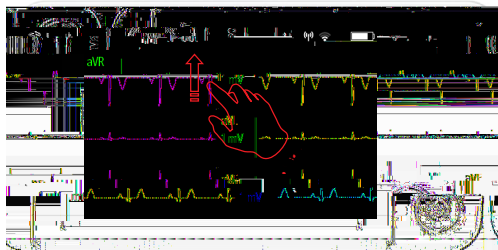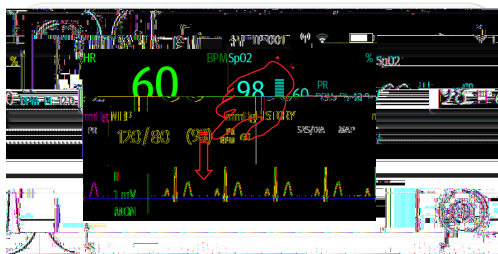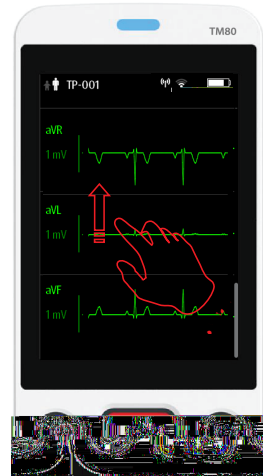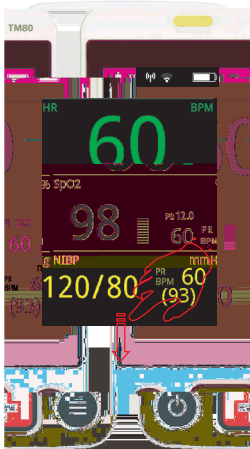

## View More Data

View More Data



## Quick Key Deployment/Screen Menu Bar Deployment



Note:

## PATIENT SETUP

### Admit

1. Tap the **Admit** button.

### Discharge

1. Tap the **Discharge** button.

2. Tap the **Discharge Patient** button.

### Note:

1. Tap the **Discharge Patient** button.

### Select the Discharge Patient menu

1. Tap the **Discharge Patient** button.

2. Tap **Discharge Patient**.

3. Tap **Yes**.

• Tap the **Discharge Patient** button.

• Tap the **Discharge Patient** button.

• Tap the **Discharge Patient** button.

1. Tap the **Discharge Patient** button.

### Adjust Patient Category

1. Tap the **Discharge Patient** button.

### Note:

1. Tap the **Discharge Patient** button.

1. Press **Menu** to display the menu.

2. Press **Menu** to display the menu.

3. Press **Patient Info**.

4. Press **Patient Category** to display the patient category.

5. Press **Yes** to confirm the patient category.

6. Press **OK** to confirm the patient category. **Patient Category**

7. Press **Menu** to display the menu.

**Note:** Press **OK** to confirm the patient category.

**Note:** Press **OK** to confirm the patient category. ( )

Press **OK** to confirm the patient category.

**Note:** Press **OK** to confirm the patient category. L, press **OK** to confirm the patient category.

L, press **OK** to confirm the patient category. L, press **OK** to confirm the patient category.

## STANDBY

### Enter Standby

1. Press **Standby** to display the standby screen.

2. Press **Standby** to display the standby screen.

3. Press **Standby** to display the standby screen.

4. Press **Standby** to display the standby screen.

5. Press **Standby** to display the standby screen. Press **Standby** to display the standby screen.

6. Press **Standby** to display the standby screen.

**Note:** Press **Standby** to display the standby screen. L, press **Standby** to display the standby screen.

L, press **Standby** to display the standby screen.

Press **Standby** to display the standby screen.

7. Press **Standby** to display the standby screen.

8. Press **Standby** to display the standby screen.

9. Press **Yes** to confirm the standby screen.





## Lead Placement

Lead placement is a critical step in the diagnostic process. The system provides a visual representation of the patient's anatomy, allowing the user to identify and mark the lead placement sites. The system uses a combination of anatomical landmarks and user input to determine the lead placement sites.

- The system uses a combination of anatomical landmarks and user input to determine the lead placement sites.


1.

- Select the **Lead Placement** option from the **Lead Placement** menu.

The system displays the lead placement sites on the patient's anatomy. The system uses a combination of anatomical landmarks and user input to determine the lead placement sites.

2. Select the **Lead Placement** option from the **Lead Placement** menu.

3. Select the **Lead Placement** option from the **Lead Placement** menu.

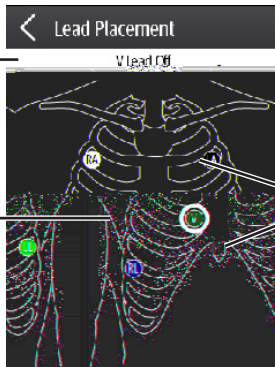


4. Select the **Lead Placement** option from the **Lead Placement** menu.

5. The system displays the lead placement sites on the patient's anatomy.

- The system uses a combination of anatomical landmarks and user input to determine the lead placement sites.
- The system uses a combination of anatomical landmarks and user input to determine the lead placement sites.
- The system uses a combination of anatomical landmarks and user input to determine the lead placement sites.





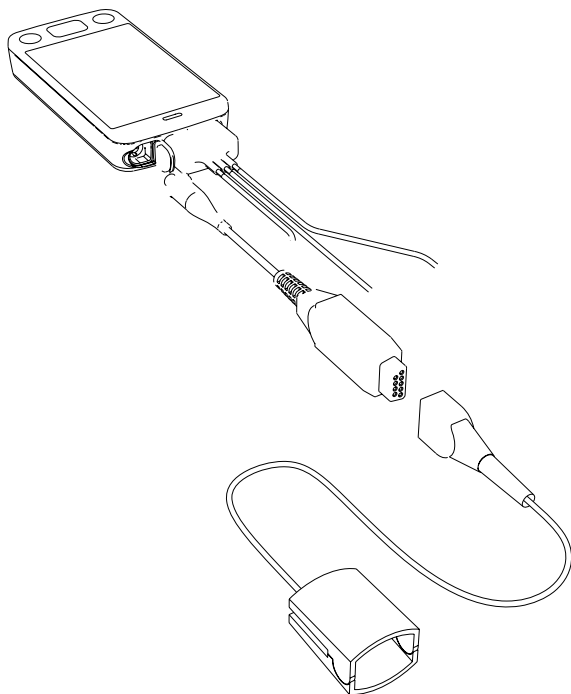

## NIBP (OPTIONAL)

1. Press **L** to enter the main menu. Press **1** to enter the **BP** menu.

### Pair a TM80 with a BP10

- 1. Press **L** to enter the main menu. Press **1** to enter the **BP** menu.
- 2. Press **2** to enter the **Pair** menu.

3. Press **1** to select **Wireless Modules.**

4. Press **1** to select **MPAN** as the **Monitor/Sensor.**

5. Press **L** to enter the main menu. Press **1** to enter the **BP** menu. Press **2** to enter the **Pair** menu. Press **1** to select **Wireless Modules.** Press **1** to select **MPAN** as the **Monitor/Sensor.** Press **1** to select **Start** to start the pairing process.

6. Press **1** to select **Connect** to connect the TM80 to the BP10. Press **1** to select **Disconnect** to disconnect the TM80 from the BP10. Press **1** to select **Connected** to confirm the connection.

7. Press **L** to enter the main menu. Press **1** to enter the **BP** menu. Press **2** to enter the **Pair** menu. Press **1** to select **Wireless Modules.** Press **1** to select **MPAN** as the **Monitor/Sensor.** Press **1** to select **Start** to start the pairing process.



8. Press **1** to select **Start** to start the pairing process. Press **1** to select **Connect** to connect the TM80 to the BP10. Press **1** to select **Disconnect** to disconnect the TM80 from the BP10. Press **1** to select **Connected** to confirm the connection.

### Pair a TM80 with a New BP10


9. Press **L** to enter the main menu. Press **1** to enter the **BP** menu. Press **2** to enter the **Pair** menu. Press **1** to select **Wireless Modules.** Press **1** to select **MPAN** as the **Monitor/Sensor.** Press **1** to select **Start** to start the pairing process.

10. Press **L** to enter the main menu. Press **1** to enter the **BP** menu. Press **2** to enter the **Pair** menu. Press **1** to select **Wireless Modules.** Press **1** to select **MPAN** as the **Monitor/Sensor.** Press **1** to select **Start** to start the pairing process.

## Unpair a TM80 with a BP10 via the TM80

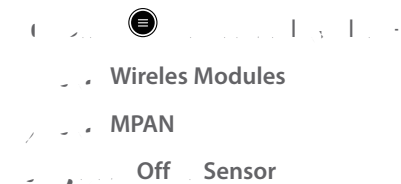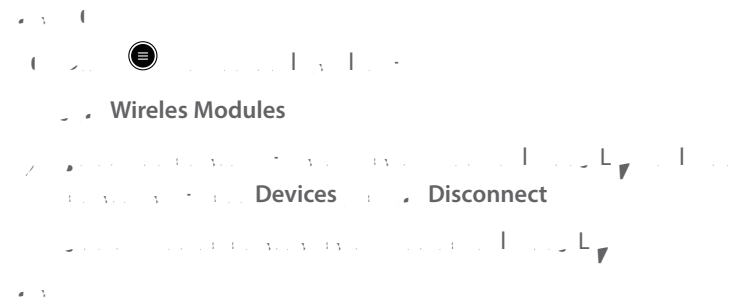

## Unpair a TM80 with a BP10 via the BP10



**Caution:** If you are using the BP10 as a remote control, you will lose control of the device.

**Caution:** If you are using the BP10 as a remote control, you will lose control of the device.

## TECHNICAL ALARMS

### Alarm Reset

Press the **Alarm Reset** button on the remote control to reset the alarm.



## Alarm Reset

When an alarm is triggered, the system will display the alarm message on the screen and sound the alarm. To reset the alarm, press the **Alarm Reset** button.

### Alarm Reset

When an alarm is triggered, the system will display the alarm message on the screen and sound the alarm. To reset the alarm, press the **Alarm Reset** button.

#### Alarm Reset

- Press the **Alarm Reset** button.
- Press the **Alarm Reset** button.
- Press the **Alarm Reset** button.
- Press the **Alarm Reset** button.

#### Alarm Reset

- Press the **Alarm Reset** button.
- Press the **Alarm Reset** button.
- Press the **Alarm Reset** button.

#### Alarm Reset

- Press the **Alarm Reset** button.
- Press the **Alarm Reset** button.

## SCREEN DISPLAY

### Switch Orientation

## Adjust Display Order

1. Press **L** to enter the menu. Use the **▲** and **▼** keys to move the cursor to the **Display** menu item. Press **▶** to enter the menu.

2. Press **▶** to enter the **Display Setup** menu.

3. Press **▶** to enter the **Display Setup** menu.

4. Press **▶** to enter the **Display Order** menu. Press **▶** to select **Portrait Order**.

5. Press **▶** to enter the **Display Order** menu. Press **▶** to select **Landscape Order**.

6. Press **▶** to enter the **Display Order** menu.

7. Press **▶** to enter the **Display Order** menu.

8. Press **▶** to enter the **Display Order** menu. Press **▶** to select **Portrait Order**.

9. Press **▶** to enter the **Display Order** menu.

10. Press **▶** to enter the **Display Order** menu.

## SCREEN LOCK/VIEW ONLY MODE

1. Press **L** to enter the menu. Use the **▲** and **▼** keys to move the cursor to the **Display** menu item. Press **▶** to enter the menu.

2. Press **▶** to enter the **Display Setup** menu.

3. Press **▶** to enter the **Display Setup** menu.

4. Press **▶** to enter the **Display Order** menu. Press **▶** to select **Portrait Order**.

5. Press **▶** to enter the **Display Order** menu. Press **▶** to select **Landscape Order**.

6. Press **▶** to enter the **Display Order** menu.

## Enable the Screen Lock

1. Press **L** to enter the menu. Use the **▲** and **▼** keys to move the cursor to the **Display** menu item. Press **▶** to enter the menu.

2. Press **▶** to enter the **Display Setup** menu.

3. Press **▶** to enter the **Display Setup** menu.

4. Press **▶** to enter the **Maintenance** menu.

5. Press **▶** to enter the **Maintenance** menu.

6. Press **▶** to enter the **Accept** menu.

7. Press **▶** to enter the **Screen Lock** menu. Press **▶** to select **Locked** or **View Only**.

8. Press **▶** to enter the **Screen Lock** menu.


9. Press **▶** to enter the **Screen Lock** menu. Press **▶** to select **Screen Lock**.

10. Press **▶** to enter the **Screen Lock** menu.


## Unlock the Screen in Locked Mode



## Unlock the Screen in View Only Mode

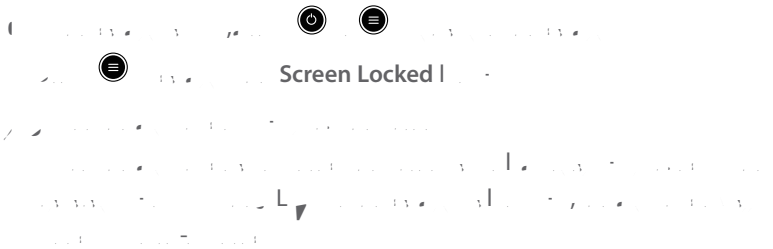

## ADJUST VOLUMES

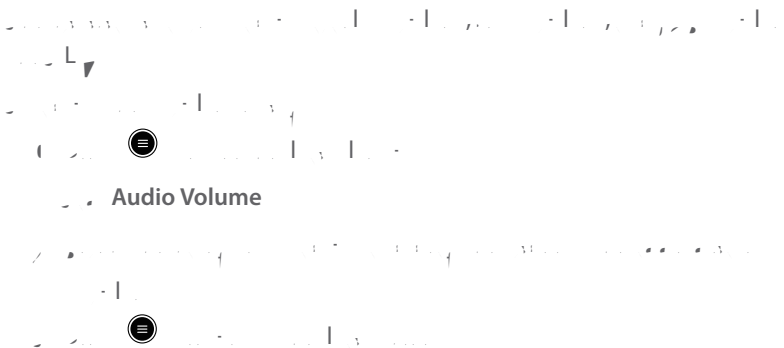

## PARAMETER COLORS

Press **L** to view the current parameter value. Press **L** again to view the parameter color (see table).

Press **L** to view the parameter color. Press **L**

to view the parameter color.

Parameter Setup

Parameter Setup

Color

Parameter Setup

Parameter Setup

**Note:** Press **L** to view the parameter value. Press **L** to view the parameter color.

## CLEAN/DISINFECT THE TM80

### Clean the TM80

Press **L** to view the parameter value. Press **L** to view the parameter color.

**Caution** Press **L** to view the parameter value. Press **L** to view the parameter color.

Press **L** to view the parameter value. Press **L** to view the parameter color.

- Press **L** to view the parameter value. Press **L** to view the parameter color.
- Press **L** to view the parameter value. Press **L** to view the parameter color.
- Press **L** to view the parameter value. Press **L** to view the parameter color.



---


# BeneVision TM80

Hand hygiene solution

Product Name	Product Type	Ingredients
BeneVision TM80	Hand hygiene solution	Ethyl alcohol 62%, Ethyl alcohol 12%, Glycerol 12%, Fragrance 0%
BeneVision TM80*		Ethyl alcohol 62%, Ethyl alcohol 12%, Glycerol 12%, Fragrance 0%
BeneVision TM80		Ethyl alcohol 62%, Ethyl alcohol 12%, Glycerol 12%, Fragrance 0%

## Notes:


 The product is not intended for use on the face, neck, or hands. It is for use on the hands only.


 The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

## Disinfect the TM80

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

## Disinfect the TM80

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

The product is not intended for use on the face, neck, or hands. It is for use on the hands only.

## **CLEAN/DISINFECT REUSABLE ACCESSORIES**

Always use appropriate cleaning and disinfection procedures for reusable accessories. Refer to the manufacturer's instructions for the specific cleaning and disinfection procedures for the accessories used with the device.

## **STERILIZATION**

Always use appropriate sterilization procedures for reusable accessories. Refer to the manufacturer's instructions for the specific sterilization procedures for the accessories used with the device.

Le...  
L...  
L...  
L...  
L...



046-011071-00(2.0)

**mindray**