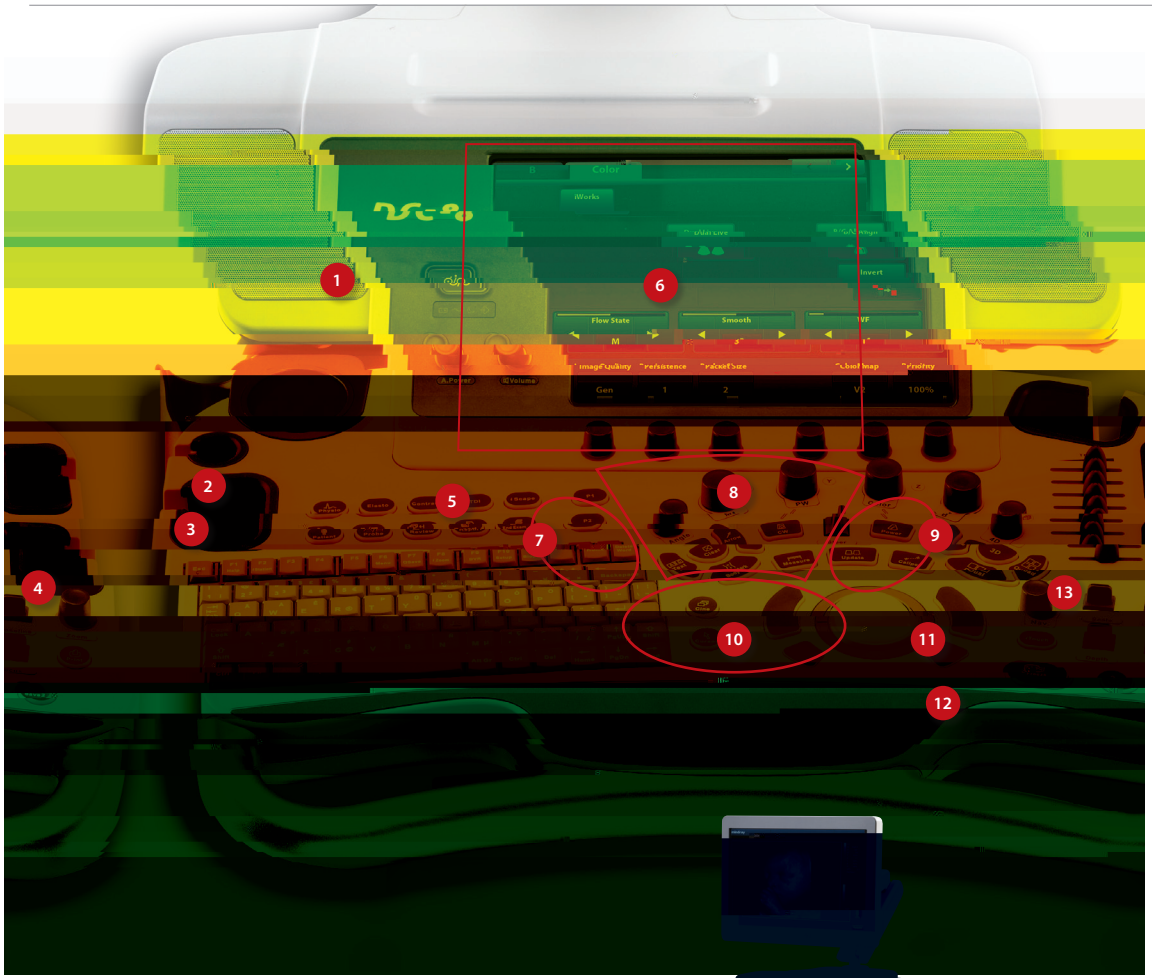

1. Power on
2. Advanced function keys
3. Exam procedure keys
4. Function key on the keyboard (F1-F12)
5. P1,P2: User-defined keys
6. Touch screen & Parameter knobs
7. Annotation
8. Imaging Mode & Measurement
9. 3D/4D: Enter/Exit 3D/4D
10. Control center
11. Optimize the image
12. Save image
13. Parameter adjustment

DC-8

Quick Reference Guide

mindray™
NORTH AMERICA

iNeedle™

One button to automatically display the needle more clear with beam steer during the biopsy process.

1. Press [iNeedle] to enter the function mode via Touch screen, parameters will be displayed on the Touch screen.

DC-8

Quick Reference Guide

Image Management

Image Transfer

1. Press [iStation™] to enter image management and select the image to send to USB, DICOM, etc.
2. Or, Press [Review] and select the image to send to USB, DICOM, etc.

Note: For detailed information, please refer to the operation manual.

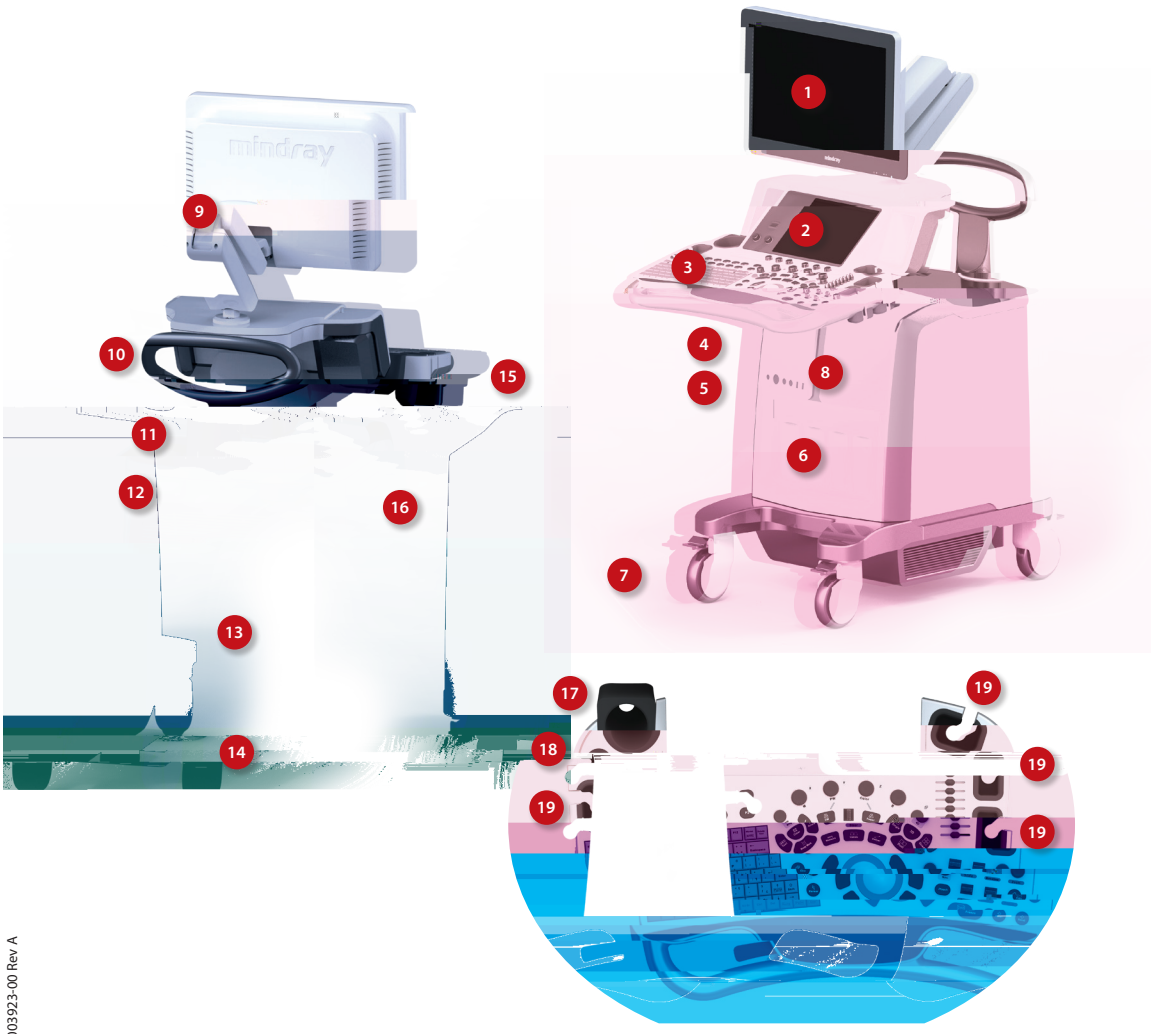

1. Monitor
2. Touch screen panel
3. Main control panel
4. Storage compartment
5. Physio panel
6. Probe sockets
7. Caster
8. Compartment
9. Articulating arm
10. Rear handle
11. Color video placing table
12. Hanger
13. I/O Panel
14. Power supply panel
15. USB_MIC port
16. DVD-RW
17. Ultrasound gel holder/gel heater
18. Pencil probe holder
19. Probe holders

P/N: 046-003923-00 Rev A

Mindray DS USA, Inc. 800 MacArthur Blvd., Mahwah, NJ 07430 Tel: 1.800.288.2121 or 201.995.8000 www.na.mindray.com