DICOM CONFORMANCE STATEMENT

FOR

M6/M6T/M6 Exp/M6s/M6 Pro/M55/M58/M5 Exp/M6Vet

DIAGNOSTIC ULTRASOUND SYSTEM

1 Conformance Statement Overview

This document describes the conformance to the ACR-NEMA DICOM 3.0 Standard by the ultrasound system of M6 Series. We specify ultrasound system generally refer to the products above in this document. The ultrasound system implements the necessary DICOM services to download worklists from an information system, save acquired Ultrasound (US) images and associated Structured Reports to a network storage device and/or removable media, print to a networked hardcopy device, query and retrieve the US images from a networked storage system, and inform the information system about the works actually done. Table 1 provides an overview of the supported network services, Table 2 lists the supported Media Storage Application Profiles, and Table 3 lists the supported Structured Report Templates.

Table 1
NETWORK SERVICES

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Transfer Storage		
Verification	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
Secondary Capture Image Storage	Yes	Yes
Query/Retrieve		
Study Root Query/Retrieve Information Model FIND	Yes	No
Study Root Query/Retrieve Information Model MOVE	Yes	No
Workflow Management		
Modality Worklist Information Model Find	Yes	No
Modality Performed Procedure Step	Yes	No
Storage Commitment Push Model	Yes	No
Print Management		
Basic Color Print Management	Yes	No
Basic Grayscale Print Management	Yes	No

8.1.2 j f i l j if d i Z m F j 73
8.1.3 Attribute Mapping..... 73
8.1.4 Coerced/Modified fields 73
8.2 Data Dictionary of private attributes 73
8.3 Coded terminology and templates..... 73
8.4 Grayscale Image Consistency..... 73
8.5 Standard extended/specialized/private sop Classes..... 74
8.6 Private Transfer Syntaxes 74
A. Appendix : OB

B.32. CID (12230) Gradient Methods....134
B.33. CID (12231) Volume Flow Methods....135
B.34. CID (12232) Myocardium Mass Methods....135
B.35. CID (12233) Cardiac Phase....135
B.36. CID (12234) Respiration Phase....135
B.37. CID (12239) Cardiac Output Properties....135
B.38. CID (12240) Left Ventricle Area....136
B.39. CID (90000) Pericardial disease....136
B.40. Mapping between Modality measurements and DICOM Concepts. 136
B.40.1. Left Ventricle Measurements....136
B.40.2. Right Ventricle Measurements....153
B.40.3. Left Atrium Measurements....154
B.40.4. Right Atrium Measurements....155
B.40.5. Aortic Valve Measurements....156
B.40.6. Mitral Valve Measurements....158
B.40.7. Pulmonic Valve Measurements....163
B.40.8. Tricuspid Valve Measurements....165
B.40.9. Aorta Measurements....167
B.40.10. Pulmonary Artery Measurements....168
B.40.11. Vena Cava Measurements....169
B.40.12. Pulmonary Venous Structure Measurements....169
B.40.13. Cardiac Shunt Study Measurements....170
B.40.14. Congenital Anomaly of Cardiovascular System Measurements....170
B.40.15. Pericardial Disease Measurements....171
B.40.16. Heart Rate Measurements....171
C. Appendix : Vascular structured reporting template....172
C.1. TID (5100) Vascular Ultrasoud Report....172
C.2. TID (1001) Observation Context....178
C.3. TID (5101) Vascular Patient Characteristics....179
C.4. TID (5102) Vascular Procedure Summary Section....180
C.5. TID (5103) Vascular Ultrasound Section....182
C.6. TID (5104) Vascular Ultrasound Measurement Group....182
C.7. CID (12104) Extracranial Arteries....183
C.8. CID (12105) Intracranial Cerebral Vessels....183
C.9. CID (12106) Intracranial Cerebral Vessels (unilateral)....184
C.10. CID (12107) Upper Extremity Arteries....184
C.11. CID (SELFCID-2) Upper Extremity Arteries(unilateral)....184
C.12. CID (12108) Upper Extremity Veins....184
C.13. CID (12109) Lower Extremity Arteries....184
C.14. CID (12110) Lower Extremity Veins....185
C.15. CID (12112) Abdominal Arteries (unilateral)....185
C.16. CID (12114) Abdominal Veins (unilateral)....186
C.17. CID (12115) Renal Vessels....186
C.18. CID (12116) Vessel Segment Modifiers....186
C.19. Mapping between Modality measurements and DICOM Concepts. 187
C.19.1. Vascular Measurements....187

C.19.2. Extracranial Arteries 187
C.19.3. Intracranial Cerebral Vessels 188
C.19.4. Intracranial Cerebral Vessels (unilateral) 188
C.19.5. Upper Extremity Arteries 188
C.19.6. Upper Extremity Arteries(unilateral) 188
C.19.7. Upper Extremity Veins 188
C.19.8. Lower Extremity Arteries 189
C.19.9. Lower Extremity Veins 189
C.19.10. Abdominal Arteries (unilateral) 190
C.19.11. Abdominal Veins (unilateral) 190
C.19.12. Renal Vessels 190

3 Introduction

3.1 Audience

This document is intended for potential customers, system integrators of medical equipment, marketing staff interested in system functionality and software designers implementing DICOM interfaces. It is assumed that the readers of this document are familiar with the DICOM Standard and with the terminology

Application Context the specification of the type of communication used between *Application Entities*. Example: DICOM network protocol.

Application Entity (AE) an end point of a DICOM information exchange, including the DICOM network or media interface software; i.e., the software that sends or receives DICOM information objects or messages. A single device may have multiple Application Entities.

Application Entity Title the externally known name of an *Application Entity*, used to identify a DICOM application to other DICOM applications on the network. The Called AE Title defines the intended receiver of an Association. Nevertheless, the Calling AE Title defines the requestor of an Association.

Application Profile - A Media Storage Application Profile defines a selection of choices at the various layers of the DICOM Media Storage Model which are applicable to a specific need or context in which the media interchange is intended to be performed.

Association a network communication channel set up between *Application Entities*.

Association Establishment - an Association Establishment is the first phase of communication between two DICOM Application Entities. The AEs use the Association Establishment to negotiate how data will be encoded and the type of data to be exchanged.

Attribute a unit of information in an object definition; a data element identified by a *tag*. The information may be a complex data structure (Sequence), itself composed of lower level data elements. Examples: Patient ID (0010,0020), Accession Number (0008,0050), Photometric Interpretation (0028,0004), Procedure Code Sequence (0008,1032).

DICOM File Format - the DICOM File Format provides a means to encapsulate in a File the Data Set representing a SOP Instance related to a DICOM Information Object.

DICOM Message Service Element (DIMSE) a DIMSE defines the services and protocols utilized by an Application Entity to exchange messages.

File - a File is an ordered string of zero or more bytes, where the first byte is at the beginning of the file and the last byte is at the end of the File. Files are identified by an unique File ID and may by written, read, or deleted.

Information Object Definition (IOD) - the specified set of *Attributes* that comprise a type of data object; does not represent a specific instance of the data object, but rather a class of similar data objects that have the same properties. The *Attributes* may be specified as Mandatory (Type 1), Required but possibly unknown (Type 2), or Optional (Type 3), and there may be conditions associated with the use of an Attribute (Types 1C and 2C). Examples: Print Job IOD.

Joint Photographic Experts Group (JPEG) a set of standardized image compression techniques, available for use by DICOM applications.

Module a set of *Attributes* within an *Information Object Definition* that are logically

Value Representation (VR) the format type of an individual DICOM data element, such as text, an integer, a persoej e d fi Zf :FD efid fef aZj can be transmitted with either explicit identification of the type of each data element (Explicit VR), or without explicit identification (Implicit VR); with Implicit VR, the receiving application must use a DICOM data dictionary to look up the format of each data element.

3.4 Acronyms, Abbreviations, and Symbols

The following acronyms and abbreviations are used in this document.

ACR	American College of Radiology
AE	Application Entity
CDR	Compact Disk Recordable
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element-Composite
FSC	File-Set Creator
FSR	File-Set Reader
FSU	File-Set Updater
HIS	Hospital Information System
IHE	Integrating the Healthcare Enterprise
IOD	Information Object Definition
ISO	International Standard Organization
JPEG	Joint Photographic Experts Group
MODALITY	Ultrasound System
MPPS	Modality Performed Procedure Step
MWL	Modality Worklist
NEMA	National Electrical Manufacturers Association
O	Optional (Key Attribute)
PACS	Picture Archiving and Communication System
PDU	Protocol Data Unit
R	Required (Key Attribute)
RIS	Radiology Information System
SCP	Service Class Provider
SCU	Service Class User
SOP	Service Object Pair
SR	Structured Reporting
TCP/IP	Transmission Control Protocol/Internet Protocol

4 Networking

4.1 Implementation Model

4.1.1 Application Data Flow

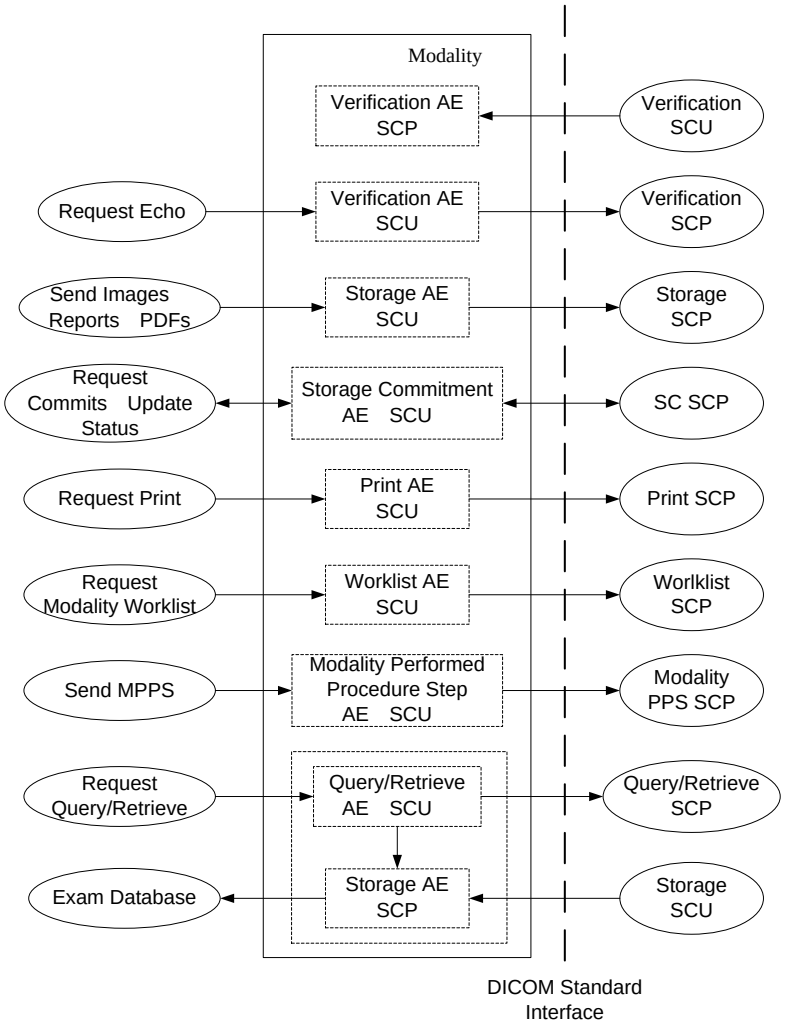

Figure 1

Implementation Model

Note Storage AE SCP only be

Operation 1

Step 1: Select the images from thumbnail menu in main UI.

g)1 i jj e f l fe e j cZ : FD fi j imZ SCPs.

Step 3: Send the image to the DICOM Storage service SCPs.

Operation 2

Step 1: Select exams in the iStation Dialog.

Step 2: Pr jj e Exam and select DICOM Storage service.

Step 3: Send the selected exams (maybe include images, SRs) to the DICOM Storage service SCPs.

Operation 3

Step 1: Select thumbnail in the iStation Dialog.

Step 2: i jj e f l fe and select DICOM Storage service SCPs.

Step 3: Send the image to the DICOM Storage service SCPs.

Operation 4

Step 1: Open the review dialog and select the images.

Step 2: Pi jj e f l fe f Z ffj j fi : j

Step 3: Send the image to the DICOM Storage service SCPs.

The SR only could be sent in the circumstance as below:

The exam type is obstetric, gynecology, cardiac, vascular,
The SR Key for the exam type must be installed in option preset UI.
Exam is the unit to send.
The status of the exam is "End", "Paused" or "Cancelled". SR would not be sent when an active exam is selected.
The DICOM storage service SCPs should be set as "Attach SR when Store Images" or "Only Store SR".

In the event that the ultrasound system is taken off the network as a portable system or when a network failure occurs during a background store, the Storage SCU maintains a queue of failed C-STORE requests. If pre-configured on Preset UI, the failed C-Store requests will be automatically retried specified times. If no pre-configuration, the user can also retry the failed requests manually.

As a SCP, the Storage AE could only be used in Query/Retrieve, otherwise couldn't.

4.1.2.3 Storage Commitment AE

The Storage Commitment AE originates associations to ensure the reliable storage of

Step 2: Prej j e f l f e e j c Z : F D print service SCPs.

Step 3: Send the image to the DICOM print service SCPs.

Operation 2

Step 1: Select exams in the iStation Dialog.

Step 2: Pr j j e Exam and select DICOM print service SCPs.

Step 3: Send the single frame images and secondary capture images of the selected exams to the DICOM print service SCPs.

Operation 3

Step 1: Select thumbnail in the iStation Dialog.

Step 2: i j j e f l f e e j c Z : F D print service SCPs.

Step 3: Send the image to the DICOM print service SCPs.

Operation 4

Step 1: Open the review dialog and select the images.

Step 2: Pi j j e f l f e f Z f f j print SCPs.

Step 3: Send the image to the DICOM print service SCPs.

4.1.2.5 Worklist AE

The Worklist AE is activated through the Worklist UI when the user selects a remote AE to query (from a pre-configured list).The system supports automatic and manual query depending on its configuration on Preset UI. The system supports fuzzy query using ? and * .

If set one and only one remote AE to be default status. The system can initiate a query with default rules when show the Worklist UI. The Worklist Server is the default server. The Modality Type is US, the Exam Date is today, and the Scheduled Station AE Title is blank.

Alternatively if the default status is no, the user can specify query rules on Worklist UI. Such as Patient ID, Patient Name, Accession Number, Requested Procedure ID, Worklist Server, Exam Date, Modality Type and Scheduled Station AE Title.

If no matches are found, a dialogue will be presented to the user to indicate so. The possible reasons for this failure are listed to help trouble shooting.

If more than one matching patients found, user can discover lists number on the UI. The user can also change query rules for another query, or for further filter in local database to locate the patients quickly. And the lists can be sorted in ascending or descending order.

4.1.2.6 MPPS AE

MPPS AE sends event transactions that facilitate the transfer of exam procedure status from the ultrasound system to the information system.

MPPS messages are sent from the system under the following circumstances:

MPPS N-Create, Status = IN PROGRESS. Starting a new exam or reactive an exam result in automated creation of an MPPS Instance managed by a remote AE.
MPPS N-Set, Status = COMPLETE. Completion of the MPPS is performed as the result of an operator action of ending the exam.
MPPS N-Set, Status = DISCONTINUED. : eZ cExam Z l j j jZfe el status to be sent. User can select various reasons from the Reason of cancel Exam UI when need to cancel an exam.

4.1.2.7 Query/Retrieve AE

The Query/Retrieve AE supports the Query/Retrieve services as an SCU.

As a Query SCU, the system initiates a C-Find request to the remote SCP if pre-configured on the Preset UI, and then query is invoked directly by the user. The system supports fuzzy query using ? and * .

For remote AE, no matter what the default status is, the user can specify query rules on Query/Retrieve UI. Such as Patient ID, Patient Name, Accession Number, Exam Date and select Search Key. If no matches are found, a dialogue will be presented to the user to indicate so. The user can also change query rules for another query, or for further filter in local database to locate the patients quickly.

As a Move SCU, the system supports the Study Root Query Model. The stystem can only retrieve ultrasound images or structed reports, whose modality atrributes are "US" or "SR", but will leap all the other ones.. Furthermore, the retrieval destination is only local host.

The system initiates a C-MOVE request to the remote Retrieve SCP when user selects items to retrieve. The remote Retrieve SCP in turn starts C-STORE sub operations to the ultrasound system.

User can discover lists number for queried items, as well as retrieval items. And the lists can be sorted in ascending or descending order.

4.1.3 Sequence of Real World Activities

All SCP activities are performed asynchronously in the background and not dependent on any sequencing.

All SCU activities are sequentially initiated in the user interface, and another activity may not be initiated until the prior activity has completed.

Application Context Name	1.2.840.10008.3.1.1.1

The PDU size is configurable with a minimum size of 16,384 and a maximum size of 65,536. The default PDU size is 32,768.

4.2.1.2.2 Number of Associations

The system initiates one Association at a time for each destination to which a transfer request is being processed in the active job queue list. Since Storage and Print tasks are executed within a same thread, when they are selected simultaneously, only one job will be active at a time, the other(s) remain pending until the active job is successful or failed.

Table 6

Number of Associations as an Association Initiator

Maximum number of simultaneous associations	1

Table 7

Number of Associations as an Association Acceptor

Maximum number of simultaneous associations	1

4.2.1.2.3 Asynchronous Nature

The ultrasound system will only allow a single outstanding operation on an association.

4.2.1.2.4 Implementation Identifying Information

Table 8

DICOM Implementation Class and Version for Modality AE

Implementation Class UID	1.2.156.112536.1.2138.0.1.0.1
Implementation Version Name	MINDRAY_V1.0

4.2.1.3 Association Initiation Policy

4.2.1.3.1 Activity Request Echo

4.2.1.3.1.1 Description and Sequencing of Activities

The user can verify the existence of a DICOM server on the hospitals network, through a

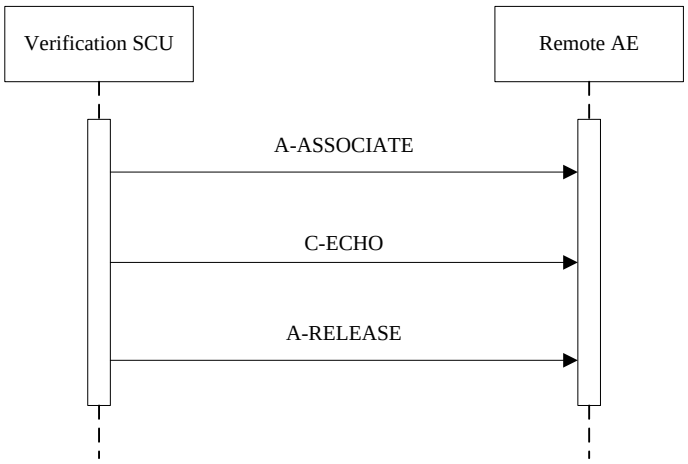

Figure 2
Sequencing of Activity Send Echo Request

4.2.1.3.1.2 Proposed Presentation Contexts

The Verification AE (as SCU) supports the following Presentation Contexts for Verification.

Table 9
Presentation Contexts for Verification

PROPOSED PRESENTATION CONTEXTS

		Value 1])			
		RLE Lossless	1.2.840.10008.1.2.5	SCU	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCU	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCU	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCU	None
		RLE Lossless	1.2.840.10008.1.2.5	SCU	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCU	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCU	None
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCU	None
		RLE Lossless	1.2.840.10008.1.2.5	SCU	None
		JPEG 2000 Image	1.2.840.10008.1.2.4.	SCU	None

	code.		send job is marked as failed. The status code is logged and the job failure is reported to the user via task management.

The behavior during communication failure is summarized in the Table below:

Table 13

Storage Communication Failure Behavior

Exception	Behavior
Timeout	The Association is aborted using A-ABORT and the send job is marked as failed. The reason is logged and the job failure is reported to the user via task management.
Association aborted by the SCP or network layers	The send job is marked as failed. The reason is logged and the job failure is reported to the user via task management.

The following table provides the list of attributes requested in the Storage.

Table 14

Storage IOD Attribute

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
Module: Patient Module (M)				
(0010,0010)	PN	2	Patient's Name	MWL/USER
(0010,0020)	LO	2	Patient ID	MWL/USER
(0010,0030)	DA	2	Patient's Birth Date	MWL/USER, default is set to zero length
(0010,0040)	CS	2	Patient's Sex	MWL/USER, default is set to zero length
(0010,1000)	LO	3	Other Patient IDs	MWL
(0010,2160)	SH	3	Ethnic Group	MWL
(0010,4000)	LT	3	Patient Comments	MWL/USER
Module: General Study Module (M)				
(0008,0020)	DA	2	Study Date	AUTO
(0008,0030)	TM	2	Study Time	AUTO
(0008,0050)	SH	2	Accession Number	MWL/USER, default is set to zero length
(0008,0090)	PN	2	Referring Physician's Name	MWL/USER, default is set to zero length
(0008,1030)	LO	3	Study Description	MWL/USER, default is set to zero length
(0008,1032)	SQ	3	Procedure Code Sequence	MWL
(0020,000D)	UI	1	Study Instance UID	MWL/AUTO
(0020,0010)	SH	2	Study ID	AUTO

Module: Patient Study Module (U)				
(0008,1080)	LO	3	Admitting Diagnoses Description	MWL
(0010,1010)	AS	3	Patient's Age	MWL/USER, default is set to zero length If the user set Patient Birth Date, it will be calculated automatically.
(0010,1020)	DS	3	Patient's Size	MWL/USER, default is set to zero length
(0010,1030)	DS	3	Patient's Weight	MWL/USER, default is set to zero length
(0010,21B0)	LT	3	Additional Patient History	MWL
Module: General Series Module (M)				
(0008,0021)	DA	3	Series Date	AUTO
(0008,0031)	TM	3	Series Time	AUTO
(0008,0060)	CS	1	Modality	
(0008,103E)	LO	3	Series Description	MWL
(0008,1050)	PN	3	Performing Physician's Name	MWL/USER, default is set to zero length
(0008,1070)	PN	3	Operators' Name	MWL/USER, default is set to zero length
(0018,1030)	LO	3	Protocol Name	AUTO set to ExamType
(0018,5100)	CS	2C	Patient Position	Set to zero length
(0020,000E)	UI	1	Series Instance UID	AUTO
(0020,0011)	IS	2	Series Number	AUTO
(0020,0060)	CS	2C	Laterality	Set to zero length
(0040,0244)	DA	3	Performed Procedure Step Start Date	MPPS
(0040,0245)	TM	3	Performed Procedure Step Start Time	MPPS
(0040,0254)	LO	3	Performed Procedure Step Description	MPPS
(0040,0260)	SQ	3	Performed Protocol Code Sequence	MPPS
Module: General Equipment Module (O)				
(0008,0070)	LO	2	Manufacturer	MINDRAY

(0008,0080)	LO	3	Institution Name	CONFIG
(0008,1010)	SH	3	Station Name	CONFIG
(0008,1040)	LO	3	Institutional Department Name	CONFIG
(0008,1090)	LO	3	Manufacturer's Model Name	M6
(0018,1000)	LO	3	Device Serial Number	The Ethernet card Mac Address
(0018,1020)	LO	3	Software Version(s)	AUTO
Module: General Image Module (M)				
(0008,0023)	DA	2C	Content Date	AUTO
(0008,0033)	TM	2C	Content Time	AUTO
(0008,2111)	ST	3	Derivation Description	CONFIG, default is set to zero length

				JPEG 2000 Image Compression (Lossless Only)
(0028,0006)	US	1C	Planar Configuration	1, if the image is sent using RLE Lossless 0 otherwise.
(0028,0009)	AT	1C	Frame Increment Pointer	Frame Time
(0028,0014)	US	3	Ultrasound Color Data Present	0 or 1
(0028,0100)	US	1	Bits Allocated	0x0008
(0028,0101)	US	1	Bits Stored	0x0008
(0028,0102)	US	1	High Bit	0x0007
(0028,0103)	US	1	Pixel Representation	0x0000
(0028,2110)	CS	1C	Lossy Image Compression	Not used if image is uncompressed; support JPEG baseline, JPEG Lossless,RLE Lossless,JPEG 2000 Image Compression,JPEG 2000 Image Compression (Lossless Only)
Module: Image Pixel Module (M)				
(0028,0010)	US	1	Rows	CONFIG
(0028,0011)	US	1	Columns	CONFIG
(0028,0034)	IS	1c	Pixel Aspect Ratio	Set to zero length
(7FE0,0010)	OW	1	Pixel Data	
Module: SOP Common Module (M)				
(0008,0005)	CS	1C	Specific Character Set	ISO_IR 100
(0008,0012)	DA	3	Instance Creation Date	AUTO
(0008,0013)	TM	3	Instance Creation Time	AUTO
(0008,0016)	UI	1C	SOP Class UID	AUTO
(0008,0018)	UI	1C	SOP Instance UID	AUTO
Module: US Region Calibration Module (U)				
(0018,6011)	SQ	1	Sequence of Ultrasound Regions	
>(0018,6012)	US	1	Region Spatial Format	Set by the system

Module: SC Equipment Module (M) Used for Second Capture Images Only				
(0008,0060)	CS	3	Modality	US
(0008,0064)	CS	1	Conversion Type	WSD
(0018,1010)	LO	3	Secondary Capture Device ID	M6
(0018,1016)	LO	3	Secondary Capture Device Manufacturer	MINDRAY
(0018,1018)	LO	3	Secondary Capture Device Manufacturer's Model Name	M6
(0018,1019)	LO	3	Secondary Capture Device Software Version(s)	AUTO

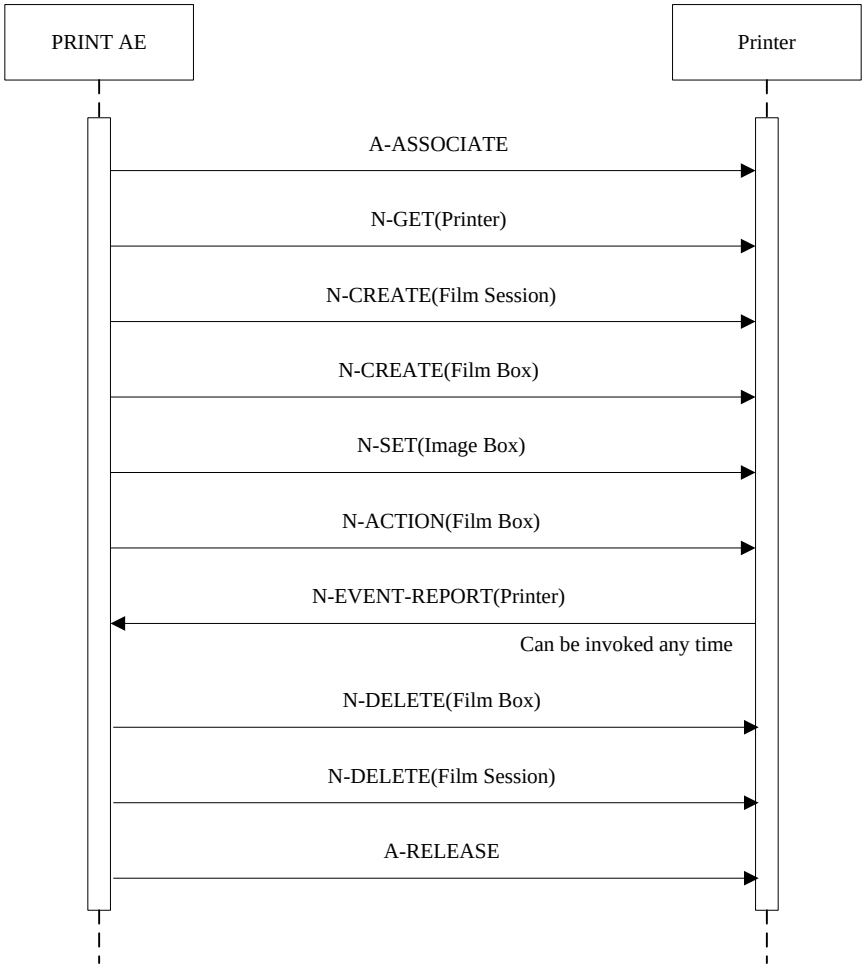

Figure 4
Sequencing of Activity Film Images

4.2.1.3.3.2 Proposed Presentation Contexts

Print AE is capable of proposing the Presentation Contexts shown in the Table below:

Table 15
Proposed Presentation Contexts for Activity Film Images

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

4.2.1.3.3.3 Common SOP Specific Conformance for all Print SOP Classes

The general behavior of Print AE during communication failure is summarized in the Table below. This behavior is common for all SOP Classes supported by Print AE.

Table 16
Print AE Communication Failure Behavior

Exception	Behavior
Timeout	The association is aborted using A-ABORT and the print-job is marked as failed.
Association aborted by the SCP or network layers	The print-job is marked as failed. The reason is logged and the job failure is reported to the user.

Recommended abbreviations to be used for the tables are:

VNAP Value Not Always Present (attribute sent zero length if no value is present)

ANAP Attribute Not Always Present

ALWAYS Always Present with a value

EMPTY Attribute is sent without a value

Recommended abbreviations to be used for the source of the data values in the tables are:

USER the attribute value source is from User input

AUTO the attribute value is generated automatically

CONFIG the attribute value source is a configurable parameter

PRINTER the attribute value is provided by printer

4.2.1.3.3.4 SOP Specific Conformance for the Printer SOP Class

Print AE supports the following DIMSE operations and notifications for the Printer SOP Class:

N-GET

N-EVENT-REPORT

Details of the supported attributes and status handling behavior are described in the following subsections.

4.2.1.3.3.4.1 Printer SOP Class Operations (N-GET)

Print AE uses the Printer SOP Class N-GET operation to obtain information about the current printer status. The attributes excepted via N-GET are listed in the Table below:

Table 17

Printer SOP Class N-GET Request Attribute Identifier List

Attribute Name	Tag
Printer Status	(2110,0010)
Printer Status Info	(2110,0020)
Printer Name	(2110,0030)
Manufacturer	(0008,0070)
Manufacturer Model Name	(0008,1090)
Device Serial Number	(0018,1000)
Software Version(s)	(0018,1020)
Date of Last Calibration	(0018,1200)
Time of Last Calibration	(0018,1201)

The behavior of Print AE when encountering status codes in a N-GET response is summarized in the Table below:

Table 18

Printer SOP Class N-GET Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The request to get printer status information was success.
Warning	any warning	xxxx	The print-job continues to be printed.
Failure	any failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.4.2 Printer SOP Class Notifications (N-EVENT-REPORT)

Table 19

Printer SOP Class N-Event-Report Behavior

Event Type Name	Event Type ID	Behavior
Normal	1	The print-job continues to be printed.
Warning	2	The print-job continues to be printed. The contents of Printer Status Info (2110, 0020) is logged and reported to the user via the job-control application.
Failure	3	The print-job is marked as failed. The contents of Printer Status Info (2110, 0020) is logged and reported to the user via the job-control

		application.
*	*	An invalid Event Type ID will cause a status code of 0113H to be returned in a N-EVENT-REPORT response.

Print AE is capable of receiving an N-EVENT-REPORT request at any time during an association. The behavior of Print AE when receiving Event Types within the N-EVENT-REPORT is summarized in the Table 19.

The reasons for returning specific status codes in a N-EVENT-REPORT response are summarized in the Table below:

Table 20

Printer SOP Class N-EVENT-REPORT Response Status Reasons

Service Status	Further Meaning	Error Code	Reasons
Success	Success	0000	The notification event has been successfully received.
Failure	No Such Event Type	0113H	An invalid Event Type ID was supplied in the N-EVENT-REPORT request.
Failure	Processing Failure	0110H	An internal error occurred during processing of the N-EVENT-REPORT. A short description of the error will be returned in Error Comment (0000, 0902).

4.2.1.3.3.5 SOP Specific Conformance for the Film Session SOP Class

Print AE supports the following DIMSE operations for the Film Session SOP Class:

N-CREATE

N-DELETE

Details of the supported attributes and status handling behavior are described in the following subsections.

4.2.1.3.3.5.1 Film Session SOP Class Operations (N-CREATE)

The attributes supplied in an N-CREATE Request are listed in the Table below:

Table 21

Film Session SOP Class N-CREATE Request Attributes

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Copies	(2000,0010)	IS	[1, 100]	ALWAYS	CONFIG
Print Priority	(2000,0020)	CS	LOW, MED,HIGH	ALWAYS	CONFIG
Medium Type	(2000,0030)	CS	BLUE FILM, CLEAR FILM, PAPER	ALWAYS	CONFIG
Film	(2000,0040)	CS	MAGAZINE PROCESSOR	ALWAYS	CONFIG

Destination					

The behavior of Print AE when encountering status codes in a N-CREATE response is summarized in the Table below:

Table 22

Film Session SOP Class N-CREATE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Memory allocation not supported	B60x	The N-CREATE operation is considered successful.
Warning	any warning	xxxx	The N-CREATE operation is considered successful.
Failure	any failure	C60x	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.5.2 Film Session SOP Class Operations (N-DELETE)

The behavior of Print AE when encountering status codes in a N-DELETE response is summarized in the Table below:

Table 23

Printer SOP Class N-DELETE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Any warning	xxxx	The N-DELETE operation is considered successful.
Failure	Any failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

following subsections.

4.2.1.3.3.6.1 Film Box SOP Class Operations (N-CREATE)

The attributes supplied in an N-CREATE Request are listed in the Table below:

Table 24
Film Box SOP Class N-CREATE Request Attributes

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Display Format	(2010,0010)	CS	PORTRAIT: STANDARD\1,1 STANDARD\1,2 STANDARD\1,3 STANDARD\2,1 STANDARD\2,2 STANDARD\2,3 STANDARD\2,4 STANDARD\3,3 STANDARD\3,4 STANDARD\3,5 STANDARD\3,6 STANDARD\4,4 STANDARD\4,5 STANDARD\4,6 STANDARD\4,7 STANDARD\4,8 STANDARD\5,5 STANDARD\5,6 STANDARD\5,7 STANDARD\5,8 STANDARD\6,6 STANDARD\6,7 STANDARD\6,8 STANDARD\6,9 STANDARD\6,10 STANDARD\7,7 STANDARD\7,8 STANDARD\7,9	ALWAYS	CONFIG

			STANDARD\7,10 STANDARD\8,8 STANDARD\8,9 STANDARD\8,10 LANDSCAPE: STANDARD\1,1 STANDARD\2,1 STANDARD\3,1 STANDARD\1,2 STANDARD\2,2 STANDARD\3,2 STANDARD\4,2 STANDARD\3,3 STANDARD\4,3 STANDARD\5,3 STANDARD\6,3 STANDARD\4,4 STANDARD\5,4 STANDARD\6,4 STANDARD\7,4 STANDARD\8,4 STANDARD\5,5 STANDARD\6,5 STANDARD\7,5 STANDARD\8,5 STANDARD\6,6 STANDARD\7,6 STANDARD\8,6 STANDARD\9,6 STANDARD\10,6 STANDARD\7,7 STANDARD\8,7 STANDARD\9,7 STANDARD\10,7 STANDARD\8,8 STANDARD\9,8		

			STANDARD\10,8		
Referenced Film Session Sequence	(2010,0500)	SQ			
>Referenced SOP Class UID	(0008,1150)	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO
>Referenced SOP Instance UID	(0008,1155)	UI	From created Film Session SOP Instance	ALWAYS	AUTO
Film Orientation	(2010,0040)	CS	PORTRAIT or LANDSCAPE	ALWAYS	CONFIG
Film Size ID	(2010,0050)	CS	8INX10IN 8_5INX11IN 10INX12IN 10INX14IN 11INX14IN 11INX17IN 14INX14IN 14INX17IN 24CMX24CM 24CMX30CM A4 A3	ALWAYS	CONFIG
Magnification Type	(2010,0060)	CS	REPLICATE, BILINEAR, CUBIC or NONE	ALWAYS	CONFIG
Max Density	(2010,0130)	US	0 .. 65535	ANAP	CONFIG
Min Density	(2010,0120)	US	0 .. 65535	ANAP	CONFIG
Trim	(2010,0140)	CS	YES or No	ALWAYS	CONFIG
Configuration Information	(2010,0150)	ST	User defined text	ANAP	USER

The behavior of Print AE when encountering status codes in a N-CREATE response is summarized in the Table below:

Table 25

Film Box SOP Class N-CREATE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Requested Min Density or Max Density outside of	B605H	The N-CREATE operation is considered successful.
Warning	Any other warning	xxxx	The N-CREATE operation is considered successful.
Failure	Any failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.6.2 Film Box SOP Class Operations (N-ACTION)

An N-ACTION Request is issued to instruct the Print SCP to print the contents of the Film Box. The Action Reply argument in an N-ACTION response is not evaluated.

The behavior of Print AE when encountering status codes in a N-ACTION response is summarized in the Table below:

Table 26

Film Box SOP Class N-ACTION Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully. The film has been accepted for printing.
Warning	Film Box SOP Instance hierarchy does not contain Image Box SOP Instances (empty page)	B603H	The N-ACTION operation is considered successful.
Warning	Image size is larger than Image Box size. The image has been demagnified.	B604H	The N-ACTION operation is considered successful.
Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609H	The N-ACTION operation is considered successful.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image or combined Print Image has been decimated to fit.	B60AH	The N-ACTION operation is considered successful.

Warning	Any other warning	xxxx	The N-ACTION operation is considered successful.
Failure	Unable to create Print Job SOP Instance; print queue is full.	C602	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Image size is larger than Image Box size.	C603	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Combined Print Image Size is larger than Image Box size.	C613	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Any other failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.6.3 Film Session SOP Class Operations (N-DELETE)

The behavior of Print AE when encountering status codes in a N-DELETE response is summarized in the Table below:

Table 27

Printer SOP Class N-DELETE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.

Warning

Details of the supported attributes and status handling behavior are described in the following subsections.

4.2.1.3.3.7.1 Image Box SOP Class Operations (N-SET)

The attributes supplied in an N-SET Request are listed in the Table below:

Table 28
Image Box SOP Class N-SET Request Attributes US

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Position	(2020,0010)	US	[1, num_image1]	ALWAYS	AUTO
Basic Grayscale Image Sequence	(2020,0111)	SQ		If the service is configured as MONOCHROME2	
>Samples Per Pixel	(0028,0002)	US	1	ALWAYS	AUTO
>Photometric Interpretation	(0028,0004)	CS	MONOCHROME2	ALWAYS	CONFIG
>Rows	(0028,0010)	US	Depends on film size	ALWAYS	AUTO
>Columns	(0028,0011)	US	Depends on film size	ALWAYS	AUTO
>Pixel Aspect Ratio	(0028,0034)	IS	Set to zero length	VNAP	AUTO
>Bits Allocated	(0028,0100)	US			

>Pixel Aspect Ratio	(0028,0034)	IS	Set to zero length	VNAP	AUTO
>Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO
>Bits Stored	(0028,0101)	US	8	ALWAYS	AUTO
>High Bit	(0028,0102)	US	7	ALWAYS	AUTO
>Pixel Representation	(0028,0103)	US	0	ALWAYS	AUTO
>Pixel Data	(7FE0,0010)	OB	Pixels of rendered film sheet	ALWAYS	AUTO

Note 1 If the attribute of Image Display Format is (STANDARD\m, n), num_image is m*n.

The behavior of Print AE when encountering status codes in a N-SET response is summarized in the Table below:

Table 29

Image Box SOP Class N-SET Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	Image print is successful, The status code is logged and the task success is reported to the user via task management.
Warning	Image size is larger than Image Box size. The image has been demagnified.	B604H	The N-SET operation is considered successful.
Warning	Requested Min Density or Max operating range.	B605H	The N-SET operation is considered successful.
Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609H	The N-SET operation is considered successful.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image or combined Print Image has been decimated to fit.	B60AH	The N-SET operation is considered successful.
Warning	Any other warning	xxxx	The N-SET operation is considered successful.
Failure	Image size is larger than Image Box size.	C603	The Association is aborted using A-ABORT and the print-job is marked as failed. The status

			meaning is logged and reported to the user.
Failure	Insufficient memory in printer to store the image.	C605	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Combined Print Image Size is larger than Image Box size.	C613	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Any other failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.4 Activity Send Find Request

4.2.1.3.4.1 Description and Sequencing of Activities

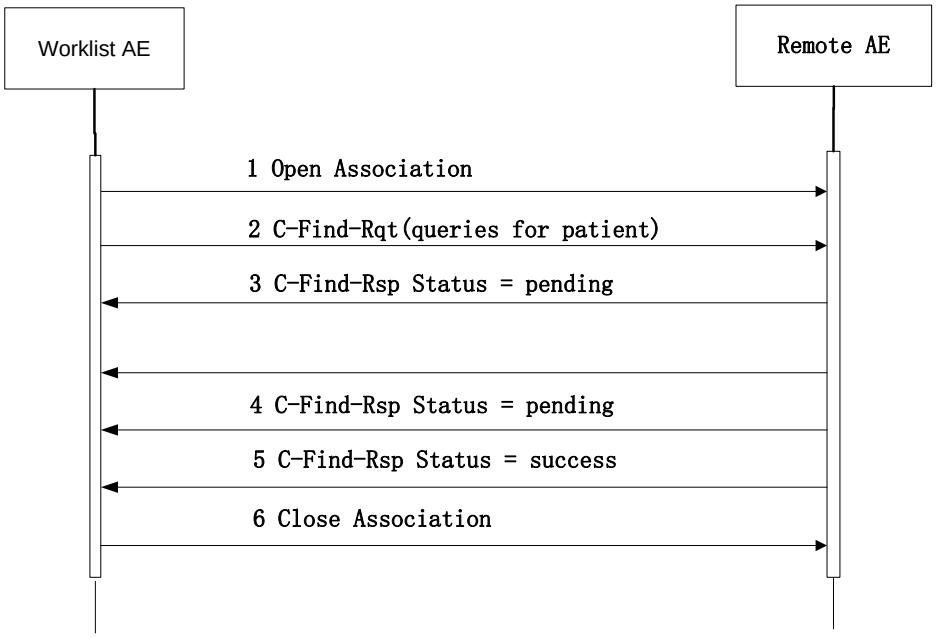

attributes.

3. The remote AE returns a C-FIND response containing the requested attributes of the first matching Item.
4. The remote AE returns another C-FIND response containing the requested attributes of the second matching Item. And then another one.
5. When the remote AE returns all the C-FIND responses with status Success indicating that no further matching Items exist.
6. The C-Find AE closes the association with the remote AE.

4.2.1.3.4.2 Proposed Presentation Contexts

Table 30
Proposed Presentation Contexts for Worklist AE

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Extended Negotiation**
Name	**UID**	**Name**	**UID**		
Modality Worklist Information Model Find	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

Worklist AE will propose Presentation Contexts for the SOP Classes listed above. For these SOP Class, Worklist AE will propose multiple Presentation Contexts, one for each of the supported Transfer Syntaxes.

If Worklist AE is offered a choice of Transfer Syntaxes in the accepted Presentation Contexts, it will apply the first encountered to use for the C-FIND operation.

4.2.1.3.4.3 SOP Specific Conformance

Table 31
C_FIND Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior (as SCU)
Refused	Out of resources	A700	The association is aborted using A-ABORT and a notify message is displayed: Some errors happen when query worklist server.
Failed	Identifier Does Not Match SOP Class	A900	
Failed	Unable to process	Cxxx	
Cancel	Matching terminated due to Cancel	FE00	/

	request		
Success	Matching is complete - No final Identifier is supplied.	0000	Patient lists show on the UI
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys.	FF00	/
Pending	Matches are continuing - Warning that one or more Optional Keys were not supported for existence for this Identifier.	FF01	/
*	The Association is aborted using A-ABORT and the query is marked as failed. The status meaning is logged and reported to the user if an interactive query. Any additional error information in the Response will be logged.	Any other status code.	The association is aborted using A-ABORT and a notify message is displayed: Some errors happen when query worklist server.

Worklist Request Identifier P

ATTRIBUTE	VR	ATTRIBUTE NAME	MATCHING KEYS	RETURN KEYS
Module: Patient Identification Module (M)				
(0010,0010)	PN	Patient's Name	configurable	X (DI)
(0010,0020)	LO	Patient ID	configurable	X(DI)
(0010,1000)	LO	Other Patient IDs		X (DI)
Module: Patient Demographic Module (M)				
(0010,0030)	DA	Patient's Birth Date		X(DI)
(0010,0032)	TM	Patient's Birth Time		X(DI)
(0010,0040)	CS	Patient's Sex		X(DI)
(0010,1020)	DS	Patient's Size		X (DI)
(0010,1030)	DS	Patient's Weight		

		Location		

Module: Visit Admission Module (M)

		Step ID		
>(0040,0010)	SH	Scheduled Station Name		X (DI)
>(0040,0011)	SH	Scheduled Procedure Step Location		X (DI)
>(0040,0012)	LO	Pre-Medication		X (DI)
> (0040,0020)	CS	Scheduled Procedure Step Status		X (DI)
> (0040,0400)	LT	Comments on the Scheduled Procedure Step		X (DI)
Module: Requested Procedure Module (M)				
(0008,1110)	SQ	Referenced Study Sequence		X (DI)
> (0008,1150)	UI	Referenced SOP Class UID		X (DI)
> (0008,1155)	UI	Referenced SOP Instance UID		X (DI)
(0020,000D)	UI	Study Instance UID		X (DI)
(0032,1060)	LO	Requested Procedure Description		X (DI)
(0032,1064)	SQ	Requested Procedure Code Sequence		X (DI)
> (0008,0100)	SH	Code Value		X (DI)
> (0008,0102)	SH	Coding Scheme Designator		X (DI)
>(0008,0103)	SH	Coding Scheme Version		X (DI)
>(0008,0104)	LO	Code Meaning		X (DI)
(0040,1001)	SH	Requested Procedure ID	configurable	X (DI)
(0040,1003)	SH	Requested Procedure Priority		X (DI)
(0040,1004)	LO	Patient Transport Arrangements		X (DI)
(0040,1400)	LT	Requested Procedure Comments		X (DI)

Module: Imaging Service Request Module (M)				
(0008,0050)	SH	Accession Number	configurable	X (DI)
(0008,0090)	PN	Referring Physician's Name		X (DI)
(0032,1032)	PN	Requesting Physician		X (DI)
(0032,1033)	LO	Requesting Service		X (DI)
(0040,2400)	LT	Imaging Service Request Comments		X (DI)
Module: SOP Common Module (M)				
(0008,0005)	CS	Specific Character Set		X (DI)
Module: Additional Attributes Module (M)				
(0008,0032)	TM	Acquisition Time		X (DI)

The convention used for Matching Keys is:

X - Return keys. An " X " indicates that MODALITY supplies this attribute as a Return Key with zero length for Universal Matching.

DI Display to the user

4.2.1.3.5 Activity Send MPPS Request

4.2.1.3.5.1 Description and Sequencing of Activities

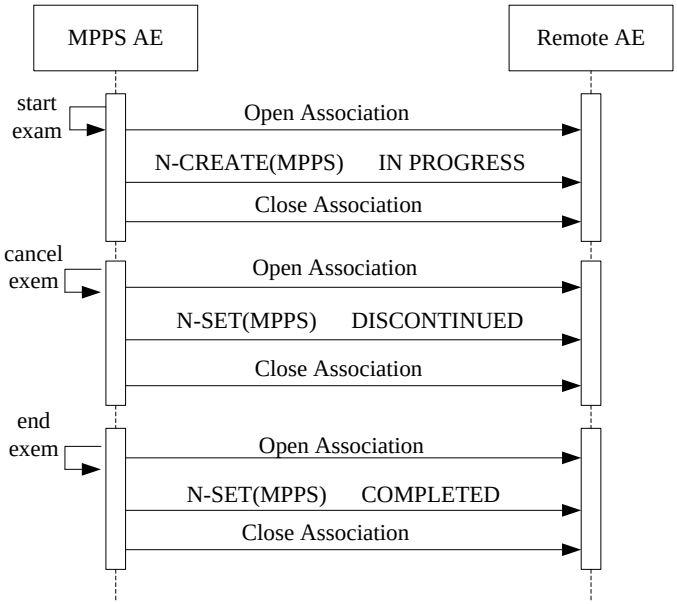

Figure 6

Sequencing of Activity MPPS progress

Note: The Cancel and End Exam commands are mutually exclusive. They are both represented here for illustration purposes only. Actual workflow uses one or the other for a

given exam.

For each exam step transfer, an attempt will be made to transmit it to the selected remote AE. If it fails, user can restart the failed task by pressing Retry Button on the DICOM task dialog.

4.2.1.3.5.2 Proposed Presentation Contexts

Table 34
Proposed Presentation Contexts for MPPS AE

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Extended Negotiation**
Name	**UID**	**Name**	**UID**		
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Failed	The association is aborted using A-ABORT and the transfer job is marked as failed. The reason is logged and reported to the user.	C60x	The association is aborted using A-ABORT and the MPPS uid isn't saved.

Table below provides a description of the MPPS N-CREATE and N-SET request identifiers sent by ultrasound system. Empty cells in the N-CREATE and N-SET columns indicate i l j ef j e e o e Z j e ggif gi m ¢ n œ j e if c e i l will be sent with zero length.

Table 36

MPPS N-CREATE / N-SET Request Identifier

Attribute Name	Tag	Req. Type N-CREATE	Req. Type N-SET
Module: Performed Procedure Step Relationship Module (M)			
Referenced Patient Sequence	(0008,1120)	2 (Default is set to null)	Not allowed
	(0010,0010)	2	Not allowed
Patient ID	(0010,0020)	2	Not allowed
	(0010,0030)	2	Not allowed
Patie	(0010,0040)	2	Not allowed
Scheduled Step Attribute Sequence	(0040,0270)	1	Not allowed
>Accession Number	(0008,0050)	2	Not allowed
>Referenced Study Sequence	(0008,1110)	2	Not allowed
>Study Instance UID	(0020,000D)	1	Not allowed
>Requested Procedure Description	(0032,1060)	2	Not allowed
>Scheduled Procedure Step Description	(0040,0007)	2	Not allowed
>Scheduled Protocol Code Sequence	(0040,0008)	2	Not allowed
>Scheduled Procedure Step ID	(0040,0009)	2	Not allowed
>Requested Procedure ID	(0040,1001)	2	Not allowed

Performed Series Sequence	(0040,0340)	2	3
>Retrieve AE Title	(0008,0054)	2 (Default is set to null)	2
>Series Description	(0008,103E)	2 (Default is set to null)	2
	(0008,1050)	2	2
	(0008,1070)	2	2
>Referenced Image Sequence	(0008,1140)	2	2
>Protocol Name	(0018,1030)	1	1
>Series Instance UID	(0020,000E)	1	1
>Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	2 (Default is set to null)	2
Module: Billing And Material Management Code Module (M)			
Billing Procedure Step Sequence	(0040,0320)	3	3
Film Consumption Sequence	(0040,0321)	3	3
Billing Supplies and Devices Sequence	(0040,0324)	3	3
Module: Performed Procedure Step Information Module (M)			
Procedure Code Sequence	(0008,1032)	2 (Default is set to null)	3
Performed Station AE Title	(0040,0241)	1	Not allowed
Performed Station Name	(0040,0242)	2 (Default is set to null)	Not allowed
Performed Location	(0040,0243)	2 (Default is set to null)	Not allowed
Performed Procedure Step Start Date	(0040,0244)	1	Not allowed
Performed Procedure Step Start Time	(0040,0245)	1	Not allowed
Performed Procedure Step End Date	(0040,0250)	2 (Default is set to null)	3
Performed Procedure Step End Time	(0040,0251)	2	3
Performed Procedure Step Status	(0040,0252)	1	3
Performed Procedure Step ID	(0040,0253)	1	Not allowed
Performed Procedure Step Description	(0040,0254)	2 (Default is set to null)	3
Performed Procedure Type Description	(0040,0255)	2 (Default is set to null)	3

Performed Procedure Step Discontinuation Reason Code Sequence	(0040,0281)	3	3
Module: SOP Common Module (M)			
Specific Character Set	(0008,0005)	1C (Required if an extended or replacement character set is used)	Not allowed

4.2.1.3.6 Activity Query/Retrieve from Remote AE

4.2.1.3.6.1 Description and Sequencing of Activities for SCU

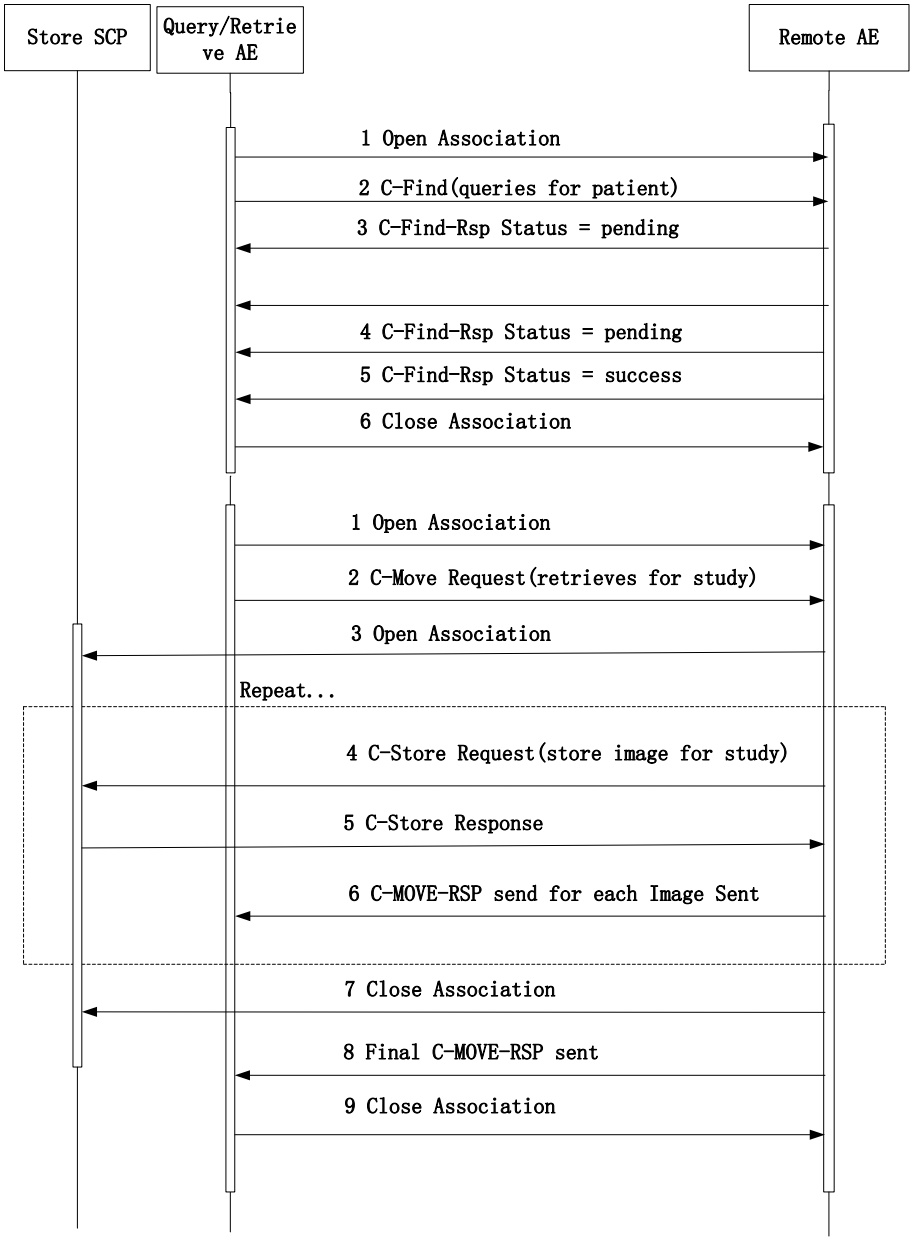

Figure 7

Sequencing of Activity Query/Retrieve progress

The associated Real-World activity is a C-Find request initiated by the user. The user

specifies some attributes the system should use to query its database. If the query user successfully establishes an association to the remote AE, it will send a C-Find request (according to the query model) and will then return the results to the application.
The C-MOVE-RQs are used to retrieve the referenced instances. The Query/Retrieve AE supports the query model Study Root.

4.2.1.3.6.2 Proposed Presentation Contexts

Table 37
Proposed Presentation Contexts for Query/Retrieve AE

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Extended Negotiation**
Name	**UID**	**Name**	**UID**		
Study Root Query/Retrieve Information Model - Find	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Study Root Query/Retrieve Information Model - Move	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

4.2.1.3.6.3 SOP Specific Conformance

The ultrasound system provides Standard Conformance to the DICOM Query/Retrieve Class.

4.2.1.3.6.3.1 Response Status

Query/Retrieve AE will behave as described in the Table below in response to the status returned in the C-Find response command message.

Table 38
C-Find Response Status Handling Behavior

Service Status	Meaning	Protocol Codes	Related Fields	Behavior (as SCU)
Refused	Refused Out of Resources	A700	(0000,0902)	The association is aborted using A-ABORT and a
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)	

	Unable to process	CXXX	(0000,0901) (0000,0902)	notify message is displayed: The remote server error.
Canceling	Matching terminated due to Cancel request	FE00	None	
Success	Matching is complete - No final Identifier is supplied	0000	None	Patient lists show on the UI
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier	/
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier	/

The ultrasound system supports the following query levels:

Study

The Query/Retrieve AE interprets following status codes

Table 39

C-Move Response Status Handling Behavior

Service Status	Meaning	Protocol Codes	Related Fields	Behavior (as SCU)
Refused	Refused Out of Resources	A700	(0000,0902)	The association is aborted using A-ABORT and a notify message is displayed: The remote server error.
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)	
	Unable to process	CXXX	(0000,0901) (0000,0902)	
Canceling	Matching terminated due to Cancel request	FE00	None	
Success	Matching is complete - No final Identifier is supplied	0000	None	Image retrieve is successful, Patient lists show on the UI

	that one or more Optional Keys were not supported for existence and/or matching for this identifier			

4.2.1.3.6.3.2 Study Root Query/Retrieve Attributes

4.2.1.3.6.3.3 Supported Matching

Following are the types of matching that can be request by the implementation:

- Single Value matching
- Universal Matching
- Wild Card Matching
- Range of date, Range of Time

The user can filter the downloaded C-FIND result, to view a limited set of the result.

4.2.1.3.6.3.4 Study Level

This section defines the keys at the Study Level of the Study Root Query/Retrieve Information Model that are supported by this implementation.

Table 40
STUDY LEVEL ATTRIBUTES

MODULE: STUDY ROOT INFORMATION MODEL (M)					
Attribute	**VR**	**Type**	**Attribute Name**	**Value**	**Matching keys**
Module: Study Root Information Model (M)					
(0008,0020)	DA	R	Study Date		DA(SK)
(0008,0030)	TM	R	Study Time		N
(0010,0010)	PN	R	Patient's Name		*(SK)
(0010,0020)	LO	R	Patient ID		S(SK)
(0008,0050)	SH	R	Accession Number		*(SK)
(0010,0030)	DA	O	Patient's Birth Date		S(SK)
(0010,0040)	CS	O	Patient's Sex		S(SK)
(0020,0010)	SH	R	Study ID		S(SK)
(0020,000D)	UI	U	Study Instance UID		N
(0008,0061)	CS	O	Modalities in Study	US	N
(0008,0090)	PN	O	Referring Physician's Name		N
(0008,1030)	LO	O	Study Description		N
(0008,1032)	SQ	O	Procedure Code Sequence		N
(0008,1060)	PN	O	Name of Physician(s) Reading Study		N
(0008,1080)	LO	O	Admitting Diagnoses Description		N
(0008,1110)	SQ	O	Referenced Study Sequence		N
(0008,1120)	SQ	O	Referenced Patient Sequence		N
(0010,0021)	LO	O	Issuer of Patient ID		N
(0010,0032)	TM	O	Patient's Birth Time		N



Table 42

COMPOSITE OBJECT INSTANCE LEVEL ATTRIBUTES

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE	MATCHINGKEYS
Module: Study Root Information Model (M)					
(0020,000D)	UI	U	Study Instance UID		S
(0020,000E)	UI	U	Series Instance UID		S
(0008,0018)	UI	U	SOP Instance UID		N
(0020,0013)	IS	R	Instance Number		N
Module: Additional Attributes Module (O)					
(0008,0016)	UI	O	SOP Class UID		N
(0008,001A)	UI	O	Related General SOP Class UID		N
(0008,3001)	SQ	O	Alternate Representation Sequence		N
>(0008,1150)	UI	O	Referenced SOP Class UID		N
>(0008,1155)	UI	O	Referenced SOP Instance UID		N
>(0020,000E)	UI	O	Series Instance UID		N
>(0040,A170)	SQ	O	Purpose of Reference Code Sequence		N
>>(0008,0100)	SH	O	Code Value		N
>>(0008,0102)	SH	O	Coding Scheme Designator		N
>>(0008,0103)	SH	O	Coding Scheme Version		N
>>(0008,0104)	LO	O	Code Meaning		N
(0040,A043)	SQ	O	Concept Name Code Sequence		N
>(0008,0100)	SH	O	Code Value		N
>(0008,0102)	SH	O	Coding Scheme Designator		N
>(0008,0103)	SH	O	Coding Scheme Version		N
>(0008,0104)	LO	O	Code Meaning		N
(0040,A504)	SQ	O	Content Template Sequence		N
>(0008,0105)	CS	O	Mapping Resource		N
>(0040,DB00)	CS	O	Template Identifier		N

4.2.1.4 Association Acceptance Policy

4.2.1.4.1 Activity Receive Echo Request

4.2.1.4.1.1 Description and Sequencing of Activities

The Verification AE (as SCP) accepts associations only if they have valid Presentation Contexts. If Verification AE (as SCP) receives an echo (C-ECHO) request then the response will be sent over the same association used to send the C-ECHO-RQ.

Figure 8

Sequencing of Activity Receive Echo Request

4.2.1.4.1.2 Accepted Presentation Contexts

It will accept Presentation Contexts as shown in the following table:

Table 43

Proposed Presentation Contex-4( )]TETB147.2.22 777.48 Tm[ltra)-3(s)6(ound)3(ex-4( )]TETB1

Table 44

Proposed Presentation Contexts for Storage

PROPOSED PRESENTATION CONTEXTS					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name**	**UID**		
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCP	None
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCP	None
Secondary	1.2.840.100	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Capture Image Storage	08.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCP	None
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None

Association aborted by the SCP or network layers	The send job is marked as failed.

4.2.1.4.3.3.2 Storage Commitment Tags (N-ACTION)

The Storage Commitment AE will request storage commitment using the following tags

NOTE: Storage Commitment may only be automatically requested upon successful completion of an end exam storage task,

Table 48

Storage Commitment N-Action-Request Message Contents

Action Type Name	Event Type ID	Attribute	Tag
N-ACTION-RQ (M)	1	Requested SOP Class UID	(0000,0003)
		Requested SOP Instance UID	(0000,1001)
Module: Additional Attributes Module (O)	3	Instance Creation Date	(0008,0012)
		Instance Creation Time	(0008,0013)
Request Storage Commitment	1	Transaction UID	(0008,1195)
		Referenced SOP Sequence	(0008,1199)
		>Referenced SOP Class UID	(0008,1150)
		>Referenced SOP Instance UID	(0008,1155)

4.2.1.4.3.3.3 Storage Commitment Notifications (N-EVENT-REPORT)

The reasons for returning specific status codes in a N-EVENT-REPORT response are summarized in the Table below.

Table 49

Storage Commitment N-EVENT-REPORT Response Status Reasons

Service Status	Further Meaning	Error Code
Success	N-EVENT-REPORT message operate success.	0000
Failed	N-EVENT- [redacted]	

4.4 Configuration

The Configuration Utility allows the service engineer to set and maintain configuration parameters of local and remote DICOM application entities.

4.4.1 AE Title/Presentation Address Mapping

This mapping (including IP and port numbers) is defined during the system Network Configuration procedure.

4.4.2 Configurable Parameters

Localhost DICOM Service Property(Including SCU and SCP):

AE Title

Port

PDU

Server Setting:

Device

IP address

Storage:

Device, Service name, AE Title and Port.

Timeout.

Maximum retries. (default value is 3)

Interval Time (In this version, this parameter is not usable.)

Compression Mode, Compression Ratio.

Color Mode (Color, Mixed, or Gray).

Cine Zoom Mode (original or 640*480)

Allow Multiframe(Enable or not)

Max Framerate(options(25, 30, 35, full), or other inputed valid value)

3D/4D(cine or volume)

SR Storage Option(Attach SR when Store Images, Only Store SR, or Not Store SR)

Default Service Status (Y/N)

Print:

Device,

STANDARD\4,6
STANDARD\4,7
STANDARD\4,8
STANDARD\5,5
STANDARD\5,6
STANDARD\5,7
STANDARD\5,8
STANDARD\6,6
STANDARD\6,7
STANDARD\6,8
STANDARD\6,9
STANDARD\6,10
STANDARD\7,7
STANDARD\7,8
STANDARD\7,9
STANDARD\7,10
STANDARD\8,8
STANDARD\8,9
STANDARD\8,10

LANDSCAPE:

STANDARD\1,1
STANDARD\1,1
STANDARD\2,1
STANDARD\3,1
STANDARD\1,2
STANDARD\2,2
STANDARD\3,2
STANDARD\4,2
STANDARD\3,3
STANDARD\4,3
STANDARD\5,3
STANDARD\6,3
STANDARD\4,4
STANDARD\5,4
STANDARD\6,4
STANDARD\7,4
STANDARD\8,4

STANDARD\5,5

STANDARD\6,5

STANDARD\7,5

STANDARD\8, 5

STANDARD\6,6

STANDARD\7,6

STANDARD\8,6

STANDARD\9,6

STANDARD\10,6

STANDARD\7,7

STANDARD\8,7

STANDARD\9,7

STANDARD\10,7

STANDARD\8,8

STANDARD\9,8

STANDARD\10,8

Destination: MAGAZINE or PROCESSOR

Film Orientation: LANDSCAPE or PORTRAIT

Priority: HIGH, MED, or LOW

Configuration Info

Magnification Type: NONE, CUBIC, REPLICATE, or BILINEAR

Trim: Yes/Not

Default Status (Y/N)

WORKLIST:

Device, Service name, AE Title and Port .

Timeout.

Maximum retries, Interval Time (In this version, these two parameters are not usable.)

Default Status (Y/N)

MPPS:

Device, Service name, AE Title and Port.

Timeout,

Maximum retries (default value is 3)

Interval Time (In this version, this parameter is not usable.)

Default Status (Y/N)

Storage Commitment:

Device, Service name, AE Title and Port.

Timeout.

Maximum retries, Interval Time (In this version, these two parameters are not usable.)

Associated Storage Service

Default Status (Not available)

Query/Retrieve

Device, Service name, AE Title and Port.

Timeout.

Maximum retries, Interval Time (In this version, these two parameters are not usable.)

Default Status (Y/N)

5 Media Storage

5.1 Implementation Model

5.1.1 Application Data Flow

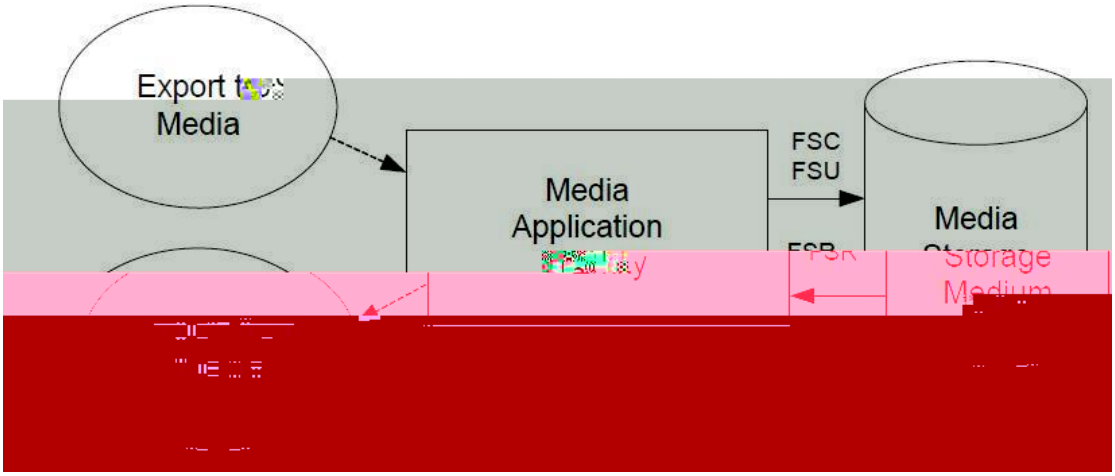

Figure 9

Application Data Flow Diagram for Media Storage

The Media Application Entity exports Images and Structured Reports to a removable storage medium. It is associated with the local real-n f i c Z m p Backup l j e configured export selection parameters for selected g e j d j e f i Structured Reports).

5.1.2 Functional

5.1.2.1 Functional Definition of Media Application Entity

j e ogf i n œg j j Z i i e œp j c Z g e j o d j f i e m l œp j c Z images to the Media Application Entity. The contents of each export job will be written to the selected media destination. The size of the selected media is used to determine and display the number of media required for the export. When a device is filled to capacity, the system will prompt the user for addition media and continue.

5.1.3 Sequencing of Real-World Activities

At least one image must exist and be selected before the Media Application Entity can be invoked. The operator can insert new media at any time. The Media Application Entity will wait indefinitely for media to be inserted before starting to write to the device.

5.1.4 File Meta Information Options

The implementation information written to the File Meta Header in each file is:

Table 52
DICOM Implementation Class and Version for Media Storage

Implementation Class UID	1.2.156.112536.1.2138.0.1.0.1
Implementation Version Name	MINDRAY_V1.0

5.2 AE Specifications

5.2.1 Media Application Entity Specification

The Media Application Entity provides standard conformance to the Media Storage Service Class. The Application Profiles and roles are listed below: The available physical media is CD-R, CD-RW, DVD-R, DVD-RW, DVD+R, DVD+RW, DVD-RAM, and USB devices.

Table 53
Application Profiles, Activities and Roles

Application Profiles Supported	Real World Activity	Role
STD-GEN-USB-JPEG STD-US-SC-SF&MF-CDR STD-US-SC-SF&MF-DVD STD-US-SC-SF&MF-DVD-RAM	Export Exam	FSC/FSU[1]
	Read Exam	FSR
	Import Exam	FSR

Note: 1 functionality requires DVD+RW, DVD-RW, or USB

5.2.1.1 File Meta Information for the Application Entity

The File Meta Header does not include the Source Application Entity Title.

5.2.1.2 Real-World Activities

5.2.1.2.1 Activity-FSC-Export exams

When system user exports exams images or SR to a media upon which no DICOM data resides, it creates a DICOM file set and writes this DICOM File Set to this media.

The Media Application Entity acts as an FSC using the interchange option when requested to export SOP Instances from the local database to media upon which no DICOM data resides.

5.2.1.2.2 Activity-FSR-Import exams

When system user presents the directory of the media, presses Restore button and the selected exams are transferred from the media to the system for review. Objects transferred to the system retain their original SOP Instance UIDs.

The Media Application Entity acts as an FSR using the interchange option when requested to import SOP Instances from media to the local database.

5.2.1.2.3 Activity-FSU-Export exams

The system user seleZj o d j ifd jpj d j i Zfip fi i ej i f d already contains data. The DICOMDIR is updated allowing access to original and new data.

The Media Application Entity acts as an FSU using the interchange option when requested to export SOP Instances from the local database to media upon which DICOM data already resides.

5.2.1.2.3.1 Media Storage Application Profiles

See Table 53 for supported Application Profiles.

5.2.1.2.3.1.1 Options

The Media Application Entity supports the SOP Classes and Transfer Syntaxes listed in the Table below:

Table 54
IODs, SOP Classes and Transfer Syntaxes

Information Object Definition	SOP Class UID	Transfer Syntax	Transfer Syntax UID
DICOM Media Storage Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian	1.2.840.10008.1.2.1
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian	1.2.840.10008.1.2.1
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian	1.2.840.10008.1.2.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1

5.3 Media Storage Application Profile

See Table 53 for supported Application Profiles.

5.3.1 DICOMDIR Attributes

The DICOMDIR file will contain the following attributes.

Table 55

Common Directory Information Module Attributes

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
(0004,1130)	CS	2	File-set ID	AUTO
(0004,1200)	UL	1	Offset of the First Directory Record of the Root Directory Entity	AUTO
(0004,1202)	UL	1	Offset of the Last Directory Record of the Root Directory Entity	AUTO
(0004,1212)	US	1	File-set Consistency Flag	0xFFFF
(0004,1220)	SQ	2	Directory Record Sequence	
>(0004,1400)	UL	1	Offset of the Next Directory Record	AUTO
>(0004,1410)	US	1	Record In-use Flag	0xFFFF
>(0004,1420)	UL	1	Offset of Referenced Lower-Level Directory Entity	AUTO
>(0004,1142)	CS	2	Specific Character Set of File-set Descriptor File	ISO_IR 100

Table 56

Patient Directory Record

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
(0004,1430)	CS	1	Directory Record Type	PATIENT
(0010,0020)	LO	1	Patient ID	MWL/USER

Table 59

Image Directory Record

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
(0004,1430)	CS	1	Directory Record Type	IMAGE
(0004,1500)	CS	1C	Referenced File ID	AUTO
(0004,1510)	UI	1C	Referenced SOP Class UID in File	AUTO
(0004,1511)	UI	1C	Referenced SOP Instance UID in File	AUTO
(0004,1512)	UI	1C	Referenced Transfer Syntax UID in File	AUTO
(0020,0013)	IS	1	Instance Number	AUTO
(0028,0008)	IS	3	Number of Frames	AUTO(Only used for mutil-frame image)

5.4 Augmented and Private Application Profiles

No augmented/private profile is supported.

5.5 Media Configuration

None.

6 SUPPORT OF CHARACTER SETS

In addition to the default character repertoire, the Defined Terms for Specific Character Set in Table 60 are supported:

Table 60
Supported Specific Character Set Defined Terms

Character Set Description	Defined Term	System Language
ISO 8859-1	ISO_IR 100	English, French, German, Italian, Portuguese, Spanish, Finnish, Danish, Icelandic, Norwegian, Swedish
ISO 8859-5	ISO_IR 144	Russian
ISO-8859-2	ISO_IR 101	Polish, Czech
ISO-8859-9	ISO_IR 148	Turkish
Chinese	GB18030	Chinese

If the system language is configured for one of above languages, the corresponding Character Set will be used automatically. Whether or not characters are displayed correctly depends on the operating system. For example, if the system is configured for Turkish, the characters of Turkish could display correctly.

7 SECURITY

7.1 Security Profiles

None supported.

7.2 Association level security

None supported.

Any Calling AE Titles and/or IP addresses may open an Association.

7.3 Application level security

None supported.

8 ANNEXES

8.1 IOD contents

8.1.1 Created SOP Instances

None.

8.1.2 Usage of attributes from received

No SOP Class specific fields are required.

The local database makes use of the conventional identification attributes to distinguish patients, studies, series and instances. In particular, if two patients have the same value for Patient ID, e s Name and Patient s Sex, they will be treated as the same in the browser and the local database.

8.1.3 Attribute Mapping

Not applicable.

8.1.4 Coerced/Modified fields

No coercion is performed.

8.2 Data Dictionary of private attributes

No private attributes are defined.

8.3 Coded terminology and templates

The value for Code Meaning will be displayed for all code sequences. No local lexicon is provided to look up alternative code meanings.

8.4 Grayscale Image Consistency

Modality does not support the Grayscale Standard Display Function.

A. Appendix : OB GYN structured reporting template

This appendix lists the DICOM Structured Report (SR) mappings used in the Obstetric and Gynecologic Structured Reports of ultrasound system SR files.

The mappings are organized in a manner similar to the DICOM SR Templates as described in PS 3.16 of the DICOM Standard. The OB-GYN Report mappings follow the DICOM SR Template TID 5000: OB-GYN Ultrasound Procedure Report, except where noted.

All private code values use the Coding Scheme Designator "MRUS".

A.1. TID (300) Measurement

This Template provides a general structure for a numeric measurement, together with evaluations of its normality and/or significance, and the inference source(s) for its value.

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			NUM	$Measurement			Units = $Units
2	>	HAS CONCEPT MOD	CODE	EV (G-C036, SRT, "Measurement Method")			$Method
3	>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")			$Derivation
4	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")			$TargetSite
5	>>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT, "Laterality")			DCID (244) Laterality

A.2. TID 1008 Subject Context, Fetus

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			PNAME	EV (121036,DCM,			
2			UIDREF	EV (121028,DCM,			
3			TEXT	EV (121030,DCM,			

4

9	>	CONTAINS	INCLUDE	DTID (5005) Fetal Biometry Section			
10	>	CONTAINS	INCLUDE	DTID (5006) Long Bones Section			
11	>	CONTAINS	INCLUDE	DTID (5007) Fetal Cranium Section			
12	>	CONTAINS	INCLUDE	DTID (5009) Fetal Biophysical Profile Section			
13	>	CONTAINS	INCLUDE	DTID (5011) Early Gestation Section			
14	>	CONTAINS	INCLUDE	DTID (5010) Amniotic Sac Section			
15	>	CONTAINS	INCLUDE	DTID (5015) Pelvis and Uterus Section			
16	>	CONTAINS	INCLUDE	DTID (5012) Ovaries Section			
17	>	CONTAINS	INCLUDE	DTID (5013) Follicles Section			$Laterality = EV (G-A101, $Number = EV (11879-4, LN, follicles in left
18	>	CONTAINS	INCLUDE	DTID (5013) Follicles Section			$Laterality = EV (G-A100, SRT, $Number = EV (11880-2, LN, follicles in right
19	>	CONTAINS	CONTAINER	EV (121070, DCM,			
20	>>	HAS CONCEPT MOD	CODE	EV (G- Finding			EV (T-F6800, SRT, Vascular

21	>>	CONTAINS	INCLUDE	DTID (5025) OB-GYN Fetal Vascular Measurement Group			$AnatomyGroup = DCID (12141) Fetal Vasculature
22	>	CONTAINS	CONTAINER	EV (121070, DCM,			
23	>>	HAS CONCEPT MOD	CODE	EV (G-			EV (T-D6007, Vascular
24	>>	CONTAINS	INCLUDE	DTID (5026) OB-GYN Pelvic Vascular Measurement Group			$AnatomyGroup = DCID (12140) Pelvic Vasculature Anatomical Location
25	>	CONTAINS	INCLUDE	DTID (SELFTMP-1)			
26	>	CONTAINS	TEXT	(20121120,MRUS, "self-defined-measurementfile")			

A.4. TID (SELFTMP-1) Fetal Cardiac Measurement Group

This is a private template referenced by TID (5000).

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	EV(T0001,MRUS,Fetel Cardiac)			
2	>	HAS OBS CONTEXT	INCLUDE	DTID (1008) Subject Context, Fetus			

A.5. TID (SELFTMP-2) Fetal Zscore

This is a private template referenced by TID (5000).

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	INCLUDE	DTID (300) Measurement			
2		CONTAINS	NUM	EV (C12017-1, MRUS, -Score by Femur			

9	>	HAS OBS CONTEXT	NUM	EV (121033,DCM,			Age (0010,1010) in Patient Study Module

A.7. TID (5001) OB-GYN Patient Characteristics

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint

6	>	CONTAINS	DATE	(11955-2, LN, "LMP"			from info
7	>	CONTAINS	DATE	33066-2, LN, "Estimated LMP by EDD"			from info
8	>	CONTAINS	DATE	11976-8, LN, "Ovulation date"			from info
9	>	CONTAINS	DATE	(I12003-01, MRUS, "IVF")			from info
10	>	CONTAINS	DATE	(C12003-01, MRUS, "EDD from IVF")			from info
11	>	CONTAINS	DATE	(I12003-02, MRUS, "PRV")			from info
12	>	CONTAINS	DATE	(C12003-02, MRUS, "EDD from PRV")			from info
13	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11886-9, LN, "Gestational Age by ovulation date")
14	>	CONTAINS	TEXT	EV (121106, DCM, Comment)			from info
15	>	CONTAINS	TEXT	(I12101-01, MRUS, "Primary Indications")			from info
16	>	CONTAINS	TEXT	(I12101-02, MRUS, "Secondary Indications")			from info
17	>	CONTAINS	TEXT	(I12101-03, MRUS, "CPT4 Code")			from info
18	>	CONTAINS	TEXT	(I12101-04, MRUS, "CPT4 Description")			from info
19	>	CONTAINS	TEXT	EV (121106, DCM, Comment)			report interface Comments
20	>						

A.9. TID (5003) OB-GYN Fetus Summary

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125008, DCM,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,"Fetus			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (18185-9, LN, "Gestational Age")
5	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11888-5, LN, " Composite Ultrasound Age")
6	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11885-1, LN, "Gestational Age
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11727-5, LN, "Estimated

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
12	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-02, MRUS, "Gestational Age by PRV")
13	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-03, MRUS, "Gestational Age by EDD")
14	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-4, MRUS, "Gestational Age by EFW")
15	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-4, MRUS, "Gestational Age by mean Gestational Sac Diameter")
16	>	CONTAINS	INCLUDE	FINDING_1			
17	>	CONTAINS	INCLUDE	FINDING_2			
18	>	CONTAINS	INCLUDE	FINDING_3			
19	>	CONTAINS	INCLUDE	FINDING_4			
20	>	CONTAINS	INCLUDE	FINDING_5			
21	>	CONTAINS	INCLUDE	FINDING_6			
22	>	CONTAINS	INCLUDE	FINDING_7			

A.10. TID (FINDING_1) Fetal Description

This is a private template referenced by TID (5003). FI

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG12019-01,MRUS,"Fetal Description")			

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
3	>	CONTAINS	TEXT	(FG7455-01,MRUS,"Gender")			
4	>	CONTAINS	TEXT	(FG7160-01,MRUS,"3 Vessel Cord")			
5	>	CONTAINS	TEXT	(T-D1200,SNM3,"Face")			
6	>	CONTAINS	TEXT	(FG4-01,MRUS,"Nose Lips")			
7	>	CONTAINS	TEXT	(FG12011-01,MRUS,"Cord insertion")			
8	>	CONTAINS	TEXT	(FG4031-01,MRUS,"LUS")			
9	>	CONTAINS	TEXT	(T-57000,SNM3,"Stomach")			
10	>	CONTAINS	CONTAINER	(T-71000,SRT,"Kidney")			
11	>>	CONTAINS	TEXT	(G-A100,SNM3,"Left")			
12	>>	CONTAINS	TEXT	(G-A101,SNM3,"Right")			
13	>	CONTAINS	TEXT	(T-74000,SRT,"Bladder")			
14	>	CONTAINS	TEXT	(T-			
15	>	CONTAINS	TEXT	(T-62000,SRT,"Liver")			
16	>	CONTAINS	TEXT	(T-D3400,SRT," Diaphragm ")			
17	>	CONTAINS	TEXT	(FG4031-02,MRUS,"Fetal Bowel")			

A.11. TID (FINDING_2) Fetus Limbs

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG4031-03,MRUS,"Fetus Limbs")			
2	>	CONTAINS	TEXT	(FG4031-04,MRUS,"Upper Extremities")			
3	>	CONTAINS	TEXT	(FG4031-05,MRUS,"Lower Extremities")			

A.12. TID (FINDING_3) Fetal Cardiology

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG4031-06,MRUS,"Fetal Cardiology")			
2	>	CONTAINS	TEXT	(FG12239-01,MRUS,"Cardiac Activity")			
3	>	CONTAINS	TEXT	(FG4031-07,MRUS,"4C HEART")			
4	>	CONTAINS	TEXT	(T-42000,SNM3,"Aorta")			
5	>	CONTAINS	TEXT	(T-44000,SNM3,Pulmonary Artery)			
6	>	CONTAINS	TEXT	(FG3010-01,MRUS,"ARCH")			
7	>	CONTAINS	TEXT	(FG3010-03,MRUS," Decrease ARCH ")			

A.13. TID (FINDING_4) Fetal Brain

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG4030-01,MRUS,"Fetal Brain")			

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
2	>	CONTAINS	TEXT	(FG4030-02,MRUS,"Lateral Ventricles")			
3	>	CONTAINS	TEXT	(11860-4,LN,"Cisterna Magna")			
4	>	CONTAINS	TEXT	(T-A600A,SNM3,"Cerebellum")			
5	>	CONTAINS	TEXT	(FG4030-03,MRUS,"CSP")			

A.14. TID (FINDING_5) Spine

This is a private template referenced by TID (5003).

NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
4	>	CONTAINS	TEXT	(FG12011-03,MRUS,"Placental Grade")			

A.16. TID (FINDING_7) Maternal Description

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG6088-01,MRUS,"Maternal Description")			
2	>	CONTAINS	CONTAINER	(FG12011-03,MRUS,"Adnexa")			
3	>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
4	>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
5	>	CONTAINS	CONTAINER	(T-87000,SRT,"Ovary")			
6	>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
7	>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
8	>	CONTAINS	CONTAINER	(T-71000,SRT,Kidney)			
9	>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
10	>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
11	>	CONTAINS	TEXT	(T-83200,SRT,Cervix)			

A.17. TID (5004)Fetal Biometry Ratio Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125001, DCM,			
2	>	HAS OBS CONTEXT	INCLUDE	EV (11951-1, LN,			

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN,			
4	>	CONTAINS	NUM	11947-9, LN, "HC/AC"			
5	>	CONTAINS	NUM	11871-1, LN, "FL/AC"			
6	>	CONTAINS	NUM	11872-9, LN, "FL/BPD"			
7	>	CONTAINS	NUM	(11823-2, LN, "Cephalic Index")			
8	>	CONTAINS	NUM	(11873-7, LN, "FL/HC")			
9	>	CONTAINS	NUM	(C12004-01, MRUS, HrtC/TC)			
10	>	CONTAINS	NUM	(C12004-02, MRUS, "TCD/AC")			
11	>	CONTAINS	NUM	(C12004-03, MRUS, LVW/HW)			
12	>	CONTAINS	NUM	(C12004-04, MRUS, "Cephalic Index by HC")			

A.18. TID (5005) Fetal Biometry Section

NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set1

							Measurements}

A.19. TID (5006) Fetal Long Bones Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125003,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (5008) Fetal Biometry Group			$BiometryType = MemberOf {DCID (12006) Fetal Long Bones Biometry Measurements}

A.20. TID (5007) Fetal Cranium Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125004,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (5008) Fetal Biometry Group			$BiometryType = MemberOf {DCID (12007) Fetal Cranium}

A.21. TID (5008) Fetal Biometry Group

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT(125005,			
2	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $BiometryType
							$Derivation = DCID (3627) Measurement Type
3	>	CONTAINS	NUM	EV (18185-9,			Units= EV (d,UCUM, days)
4	>>	INFERRED FROM	CODE	DCID (228) Equation or Table			DCID (12013) Gestational Age Equations and Tables
5	>>	R-INFERRED FROM	NUM				
6	>>	HAS PROPERTIES	NUM	DCID (226) Population Statistical Descriptors			
7	>	CONTAINS	NUM	(DCM, 125012, "Growth Percentile Rank")			
8	>>	INFERRED FROM	CODE	DCID (228) Equation or Table			

A.22. TID (5009) Fetal Biophysical Profile Section

	NL	Relation with Parent	Value Type	Concept Name	Used in Modality	Condition	Value Set Constraint
1			CONTAINER	DT (125006,			

EV (11951-1,LN,			
EV (11878-6,LN, "Number of			
EV (11631-9, LN,			Units = DT
(121106, DCM,			
EV (11632-7, LN,			Units = DT

A.23. TID (5010) Amniotic Sac Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (121070, DCM,)			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3,			DT (T-F1300,
3	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = DT (11627-7, LN,
4	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11624-4, LN,
5	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11626-9, LN, Second Quadrant
6	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11625-1, LN, ant
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11623-6, LN, "Fourth Quadrant
8	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (M12008-01,MRUS, "Amniotic Fluid")

A.24. TID (5011) Early Gestation Section

	NL	Relation	Value Type	Concept	Used in	Condition	Value Set

5	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11840-
6	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11857-
7	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (12164-
8	>	CONTAINS	INCLUDE	EV (T-87000,			$GroupName = EV (T-
9	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11830-
10	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11841-
11	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11858-
12	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (12165-

A.26. TID (5013) Follicles Section

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (121070, DCM,			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3,			DT (T-87600, SRT,

5	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (M11793-01, LN,
6	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (M11794-01, MRUS,
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11793-7, LN

A.28. TID (5015) Pelvis And Uterus Section

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125011,			
2	>	CONTAINS	CONTAINER	$GroupName			$GroupName = EV (T-
3	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Width $Width = EV (11865-
4	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Length $Length = EV (11842-2,
5	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Height $Height = EV (11859-6,
6	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Volume $Volume = EV (33192-6,
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV(LN,11961-0,Cervix Length)
8	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV(LN,12145-9,Endometrium Thickness)

	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,M12011-01,Cervix Height)
	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,M12011-02,Cervix Width)
	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,C12011-03,Uterus Body)
	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,C12011-04,UT_L/CX_L)
	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,M12011-03,Matrix Kindney Length)

.29. TID (5025) OB-GYN Fetus Vascular Ultrasound Measurement Group

	Rel with Parent	**VT**	**Concept Name**	**Used in MODALITY**	**Condition**	**Value Set Constraint**
		CONTAINER	$AnatomyGroup			
2 >	HAS CONTEXT	OBS	TEXT	EV (11951-1,LN,		

A.30. TID (5026) OB-GYN Pelvic Vascular Ultrasound Measurement Group

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	$AnatomyGroup			
2	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT,			DCID (244) Laterality
3	>	HAS CONCEPT MOD	TEXT	(112050, DCM,			
4	>	CONTAINS	INCLUDE	DTID (300) Measurement	√		$MeasType = DCID (12119) Vascular Ultrasound Property $Derivation = DCID (3627) Measurement Type

A.31. CID (228) Equation or Table

CSD	CV	Code Meaning
DCM	121420	Equation
DCM	121421	Equation Citation
DCM	121424	Table of Values
DCM	121422	Table of Values Citation
DCM	121423	Method Citation

A.32. CID (244) Laterality

CSD	CV	Code Meaning
SRT	G-A100	Right
SRT	G-A101	Left
SRT	G-A102	Right and left
SRT	G-A103	Unilateral

A.33. CID (3627) Measurement Type

CSD	CV	Code Meaning

SRT	R-002E1	Best value
SRT	R-00317	Mean
SRT	R-00319	Median
SRT	R-0032E	Mode
SRT	R-00355	Point source measurement
SRT	R-00353	Peak to peak
SRT	R-41D27	Visual estimation
SRT	R-10260	Estimated
SRT	R-41D2D	Calculated
SRT	R-41D41	Measured

A.34. CID (12005) Fetal Biometry Measurements

CSD	CV	Code Meaning
LN	11979-2	Abdominal Circumference
LN	11818-2	Anterior-Posterior Abdominal Diameter
LN	11819-0	Anterior-Posterior Trunk Diameter
LN	11820-8	Biparietal Diameter
LN	11860-4	Cisterna Magna
LN	11963-6	

A.35. CID (12006) Fetal Long Bones Measurements

CSD	CV	Code Meaning
LN	11966-9	Humerus length
LN	11967-7	Radius length
LN	11969-3	Ulna length
LN	11968-5	Tibia length
LN	11964-4	Fibula length
LN	11962-8	Clavicle length
LN	11963-6	Femur Length

A.36. CID (12007) Fetal Cranium

CSD	CV	Code Meaning
LN	12171-5	Lateral Ventrical width
LN	11860-4	Cisterna Magna length
LN	12146-7	Nuchal Fold thickness
LN	33070-4	Inner Orbital Diameter
LN	11629-3	Outer Orbital Diameter
LN	11863-8	Trans Cerebellar Diameter
LN	33069-6	Nuchal Translucency
LN	12170-7	Width of Hemisphere
MRUS	M12007-01	Ear Length
MRUS	M12007-02	Middle Phalanx Length
MRUS	M12007-03	Orbit
MRUS	M12007-04	OFDHC
MRUS	C12007-01	HCc

A.37. CID (12009) Early Gestation Biometry Measurements

CSD	CV	Code Meaning
LN	11957-8	Crown Rump Length
LN	11850-5	Gestational Sac Diameter
LN	33071-2	Spine Length

LN	11816-6	Yolk Sac length
LN	33069-6	Nuchal Translucency
MRUS	C12009-01	Mean Gestational Sac Diameter
MRUS	M12009-01	Gestational Sac Diameter1
MRUS	M12009-02	Gestational Sac Diameter2
MRUS	M12009-03	Gestational Sac Diameter3

A.38. CID (12013) Gestational Age Equations and Tables

CSD CV

CSD	CV	Code Meaning
LN	11936-2	

CSD

CSD	CV	Code Meaning
MRUS	F12013-41	CUA by BPD, HC, AC, FL, Hadlock 1984
MRUS	F12014-01	EFW by AC,BPD,Merz 1991
MRUS	F12014-02	EFW by AC,Merz 1991
MRUS	F12014-03	EFW by BPD, TTD, Hansmann 1995
MRUS	F12014-04	EFW by BPD, FTA, FL, Osaka 1983
MRUS	F12014-05	EFW by AC,HC,FL,Schild 2004
MRUS	F12014-06	EFW by BPD,FL,MAD,Persson 1996

A.40. CID (12015) Fetal Growth Equations and Tables

CSD	CV	Code Meaning
LN	33146-2	AC by GA, Hadlock 1984
LN	33546-3	AC (derived) by GA, Chitty 1994
LN	33198-3	BPD by GA, Hadlock 1984
LN	33152-0	outer-outer by GA, Chitty 1994
LN	33155-3	BPD by GA, Rempen 1991
LN	33160-3	CRL by GA, Rempen1991
LN	33166-0	FL by GA, Hadlock 1984
LN	33167-8	FL by GA, Chitty 1994
LN	33171-0	GS by GA, Rempen 1991
LN	33173-6	HC by GA, Hadlock 1984
LN	33174-4	HC derived by GA, Chitty 1994
LN	33181-9	TCD by GA Goldstein 1987
LN	33097-7	Fibula, Jeanty 1983
LN	33126-4	Radius, Jeanty 1983
MRUS	F12015-01	AC by GA, ASUM 2001
MRUS	F12015-02	AC by GA, Merz 1991
MRUS	F12015-03	AC, Jeanty 1984
MRUS	F12015-04	APAD,Merz 1991
MRUS	F12015-05	BPD by GA, ASUM 2001
MRUS	F12015-06	BPD, Hansmann 1985
MRUS	F12015-07	BPD by GA, Merz 1988
MRUS	F12015-08	BPD,Kurtz,1980
MRUS	F12015-09	BPD,Sabbagha 1978
MRUS	F12015-10	BPD, Tokyo 1989

CSD	CV	Code Meaning
MRUS	F12015-12	

CSD	CV	Code Meaning
INCLUDE	CID 12121 Vascular Indices and Ratios	
INCLUDE	CID 12122 Other Vascular Properties	

A.42. CID (12120) Blood Velocity Measurements

CSD	CV	Code Meaning
LN	11653-3	End Diastolic Velocity
LN	11665-7	Minimum Diastolic Velocity
LN	11726-7	Peak Systolic Velocity
LN	11726-7	Peak Velocity
LN	20352-1	Time averaged mean velocity
LN	11692-1	Time averaged peak velocity

A.43. CID (12121) Vascular Indices and Ratios

CSD	CV	Code Meaning
LN	12008-9	Pulsatility Index
LN	12023-8	Resistivity Index
LN	12144-2	Systolic to Diastolic Velocity Ratio
MRUS	M12119-04	Diastolic to Systolic Velocity Ratio
MRUS	C12121-1	Systolic to Atrial Contraction Velocity Ratio
MRUS	M12120-1	Peak Early Diastolic Velocity
MRUS	C12121-2	Peak velocity index for the vein

A.44. CID (12122) Other Vascular Properties

CSD	CV	Code Meaning
LN	20168-1	Acceleration Time
LN	20217-6	Deceleration Time
SRT	R-1025C	Vessel Intimal Diameter
LN	20247-3	Peak Gradient
LN	20256-4	Mean Gradient
LN	20354-7	Velocity Time Integral
LN	11948-7	Fetal Heart Rate
LN	8867-4	Heart rate
MRUS	M12119-02	Angle

MRUS	M12119-01	Mean Velocity Mean Pressure Gradient
MRUS	M12119-06	Vol Flow(TAMAX)
MRUS	M12119-07	Vol Flow(TAMEAN)

A.45. CID (12140) Pelvic Vasculature Anatomical Location

CSD	CV	Code Meaning
SRT	T-46980	Ovarian Artery
SRT	T-46820	Uterine Artery

A.46. CID (12141) Fetal Vasculature Anatomical Location

CSD	CV	Code Meaning
SRT	T-42000	Aorta
SRT	T-D0765	Descending Aorta
SRT	T-45600	Middle Cerebral Artery
MRUS	V12141-01	Ductus Venosus
SRT	T-F1810	Umbilical Artery
SRT	T-F1820	Umbilical Vein
SRT	T-F1412	Vitelline Artery of Placenta

A.47. CID (SELFCID-1) Fetal Z-Score

CSD	CV	Code Meaning
LN	12204-06	Aortic Valve Diameter
LN	18012-5	Ascending Aortic Diameter
LN	18013-3	Descending Aortic Diameter
LN	18019-0	Left Pulmonary Artery Diameter
LN	18021-6	Right Pulmonary Artery Diameter
LN	18020-8	Main Pulmonary Artery Diameter
LN	18154-5	Interventricular Septum Diastolic Thickness
LN	18158-6	Interventricular Septum Systolic Thickness
MRUS	M12204-06	Aortic Valve Diameter(Z Score)
MRUS	M18020-8	Main Pulmonary Artery Diameter(Z Score)
MRUS	C12201-06	Left Ventricular Diameter/Right Ventricular Diameter
MRUS	C12201-07	Left Ventricular Diameter/Right Ventricular Diameter(Z Score)
MRUS	C12205-03	Left Atrium Diameter / Right Atrium Diameter
MRUS	C12205-04	Left Atrium Diameter / Aorta Diameter

MRUS	C12205-05	Left Atrium Diameter / Aorta Diameter(Z Score)
MRUS	C12212-01	Aorta Diameter/Main Pulmonary Artery Diameter
MRUS	C12212-03	Aorta Diameter/Main Pulmonary Artery Diameter(Z Score)
MRUS	M12201-01	Left ventricular short-axis diameter at end diastole
MRUS	M12201-08	Left ventricular short-axis diameter at end diastole(Z Score)
MRUS	M12201-02	Left ventricular short-axis diameter at end systole
MRUS	M12201-03	Left ventricular Diameter
MRUS	M12201-09	Left ventricular Diameter(Z Score)
MRUS	M12201-04	interventricular septal thichness
MRUS	M12201-05	Left Ventricular Outflow Tract Diameter
MRUS	M12204-01	Right ventricular short-axis diameter at end diastole
MRUS	M12204-07	Right ventricular short-axis diameter at end diastole(Z Score)
MRUS	M12204-02	Right ventricular short-axis diameter at end systole
MRUS	M12204-03	Right ventricular Diameter
MRUS	M12204-08	Right ventricular Diameter(Z Score)
MRUS	M12204-09	Right ventricular area(Z Score)
MRUS	M12204-04	Right ventricular area
MRUS	M12206-01	Right Atrium Diameter
MRUS	M12204-05	Right Ventricular Outflow Tract Diameter
MRUS	M12205-01	Left Atrium Diameter
MRUS	M12205-02	Left Atrium area
MRUS	M12206-02	Right Atrium area
MRUS	M12240-01	Left ventricular area
MRUS	M12240-02	Left ventricular area(Z Score)
MRUS	M12209-1	Pulmonary Valve Diameter(Z Score)
MRUS	M12215-1	Inferior Vene Cava Diameter(Z Score)
MRUS	M12212-1	Duct Aorta Diameter(Z Score)
MRUS	M12208-1	Tricuspid Valve Diameter(Z Score)
MRUS	M12207-1	Mitral Valve Diameter(Z Score)

MODALITY Label	***DICOM Mapping***
HUM	11966-9,LN,Humerus length
RAD	11967-7,LN,Radius length
Ulna	11969-3,LN,Ulna length
Tibia	11968-5,LN,Tibia length
FIB	11964-4,LN,Fibula length
CLAV	11962-8,LN,Clavicle length
LVW	12171-5,LN,Lateral Ventrical width
NF	12146-7,LN,Nuchal Fold thickness
IOD	33070-4,LN,Inner Orbital Diameter
OOD	11629-3,LN,Outer Orbital Diameter
TCD	11863-8,LN,Trans Cerebellar Diameter
NT	33069-6,LN,Nuchal Translucency
HW	12170-7,LN,Width of Hemisphere
Ear	M12007-01,MRUS,Ear Length
MP	M12007-02,MRUS,Middle Phalanx Length
Orbit	M12007-03,MRUS,Orbit
OFD(HC)	M12007-04,MRUS,OFDHC
HC(c)	C12007-01,MRUS,HCc
AF1	11624-4,LN,First Quadrant Diameter
AF2	11626-9,LN,Second Quadrant Diameter
AF3	11625-1,LN,Third Quadrant Diameter
AF4	11623-6,LN,Fourth Quadrant Diameter
AF	M12008-01,MRUS,Amniotic Fluid
CRL	11957-8,LN,Crown Rump Length
GS	11850-5,LN,Gestational Sac Diameter
Vertebrae	33071-2,LN,Spine Length
YS	11816-6,LN,Yolk Sac length
NT	33069-6,LN,Nuchal Translucency
Mean Sac Diam	C12009-01,MRUS,Mean Gestational Sac Diameter
Cervix L	11961-0,LN,Cervix Length
Cervix L	11961-0,LN,Cervix Length
Endo	12145-9,LN,Endometrium Thickness
Cervix H	M12011-01,MRUS,Cervix Height
Cervix W	M12011-02,MRUS,Cervix Width

MODALITY Label	***DICOM Mapping***
Uterus Body	C12011-03,MRUS,Uterus Body
UT-L/CX-L	C12011-04,MRUS,UT_L/CX_L
Mat Kidney	M12011-03,MRUS,Matrix Kindney Length
AFI	11627-7,LN,Amniotic Fluid Index
Ovary W	11829-9, LN, Left Ovary Width;11830-7, LN, Right Ovary Width
Ovary L	11840-6, LN, Left Ovary Length;11841-4, LN, Right Ovary Length
Ovary H	11857-0, LN, Left Ovary Height;11858-8, LN, Right Ovary Height
Ovary Vol	12164-0, LN, Left Ovary Volume;12165-7, LN, Right Ovary Volume
Follicle1 L	M11793-02, MRUS, Follicle Length
Follicle2 L	M11793-02, MRUS, Follicle Length
Follicle3 L	M11793-02, MRUS, Follicle Length
Follicle4 L	M11793-02, MRUS, Follicle Length
Follicle5 L	M11793-02, MRUS, Follicle Length
Follicle6 L	M11793-02, MRUS, Follicle Length
Follicle7 L	M11793-02, MRUS, Follicle Length
Follicle8 L	M11793-02, MRUS, Follicle Length
Follicle9 L	M11793-02, MRUS, Follicle Length
Follicle10 L	M11793-02, MRUS, Follicle Length
Follicle11 L	M11793-02, MRUS, Follicle Length
Follicle12 L	M11793-02, MRUS, Follicle Length
Follicle13 L	M11793-02, MRUS, Follicle Length
Follicle14 L	M11793-02, MRUS, Follicle Length
Follicle15 L	M11793-02, MRUS, Follicle Length
Follicle16 L	M11793-02, MRUS, Follicle Length
UT W	11865-3,LN,Uterus Width
UT L	11842-2,LN,Uterus Length
UT H	11859-6,LN,Uterus Height
UT Vol	33192-6,LN,Uterus Volume
Follicle1 W	M11793-01,MRUS,Follicle Width
Follicle2 W	M11793-01,MRUS,Follicle Width
Follicle3 W	M11793-01,MRUS,Follicle Width
Follicle4 W	M11793-01,MRUS,Follicle Width
Follicle5 W	M11793-01,MRUS,Follicle Width
Follicle6 W	M11793-01,MRUS,Follicle Width

MODALITY Label	*DICOM Mapping*
Follicle9 Diam	11793-7,LN,Follicle Diameter
Follicle10 Diam	11793-7,LN,Follicle Diameter
Follicle11 Diam	11793-7,LN,Follicle Diameter
Follicle12 Diam	11793-7,LN,Follicle Diameter
Follicle13 Diam	11793-7,LN,Follicle Diameter
Follicle14 Diam	11793-7,LN,Follicle Diameter
Follicle15 Diam	11793-7,LN,Follicle Diameter
Follicle16 Diam	11793-7,LN,Follicle Diameter
EFW1	11727-5,LN,Estimated Weight
EFW2	11727-5,LN,Estimated Weight
CP	11767-1,LN EFW percentile rank
UP	11767-1,LN EFW percentile rank
CP	11767-1,LN EFW percentile rank
UP	11767-1,LN EFW percentile rank
EFW(Campbell)	11727-5,LN,Estimated Weight
EFW(Hadlock1)	11727-5,LN,Estimated Weight
EFW(Hadlock2)	11727-5,LN,Estimated Weight
EFW(Hadlock3)	11727-5,LN,Estimated Weight
EFW(Hadlock4)	11727-5,LN,Estimated Weight
EFW(Hansmann)	11727-5,LN,Estimated Weight
EFW(Merz1)	11727-5,LN,Estimated Weight
EFW(Merz2)	11727-5,LN,Estimated Weight
EFW(Osaka)	11727-5,LN,Estimated Weight
EFW(Shepard)	11727-5,LN,Estimated Weight
EFW(Tokyo)	11727-5,LN,Estimated Weight
EFW(Schild)	11727-5,LN,Estimated Weight
EFW(Persson)	11727-5,LN,Estimated Weight
PL Thickness	M12011-01,MRUS,Placental Thickness
Sac Diam1	M12009-01,MRUS,Gestational Sac Diameter1
Sac Diam2	M12009-02,MRUS,Gestational Sac Diameter2
Sac Diam3	M12009-03,MRUS,Gestational Sac Diameter3

A.48.2. Vasculature Anatomic Location

MODALITY Vasculature Anatomic Location	*DICOM Mapping*
Ovarian A	T-46980, SRT, Ovarian Artery
Ut A	T-46820, SRT, Uterine Artery
Fetal Ao	T-42000, SRT, Aorta
Desc Aorta	T-D0765, SRT, Descending Aorta
MCA	T-45600, SRT, Middle Cerebral Artery
Duct Veno	V12141-01, MRUS, Ductus Veno
Umb A	T-F1810, SRT, Umbilical Artery
Umb V	T-F1820, SRT, Umbilical Vein
Placenta A	T-F1412, SRT, Vitelline Artery of Placenta

A.48.3. OB-GYN Vascular Measurements

MODALITY Label	*DICOM Mapping*
<Vasculature Anatomic Location> ED	11653-3, LN, End Diastolic Velocity
<Vasculature Anatomic Location> MD	11665-7 , LN, Minimum Diastolic Velocity
<Vasculature Anatomic Location> PS	11726-7, LN, Peak Systolic Velocity
<Vasculature Anatomic Location> TAMEAN	20352-1, LN, Time averaged mean velocity
<Vasculature Anatomic Location> TAMAX	11692-1, LN, Time averaged peak velocity
<Vasculature Anatomic Location> PV	11726-7, LN, Peak Velocity
<Vasculature Anatomic Location> PI	12008-9, LN, Pulsatility Index
<Vasculature Anatomic Location> RI	12023-8, LN, Resistivity Index
<Vasculature Anatomic Location> S/D	12144-2, LN, Systolic to Diastolic Velocity Ratio
<Vasculature Anatomic Location> D/S	M12119-04, MRUS, Diastolic to SystolicVelocity Ratio
<Vasculature Anatomic Location> D	M12120-1,MRUS, Peak Early Diastolic Velocity
<Vasculature Anatomic Location> PVIV	C12121-2,MRUS,Peak velocity index for the vein
<Vasculature Anatomic Location> AT	20168-1, LN, Acceleration Time
<Vasculature Anatomic Location> DT	20217-6, LN, Deceleration Time
<Vasculature Anatomic Location> PPG	20247-3, LN, Peak Gradient
<Vasculature Anatomic Location> MPG	20256-4, LN, Mean Gradient
<Vasculature Anatomic Location> MMPG	M12119-01, MRUS, Mean Velocity Mean Pressure Gradient
<Vasculature Anatomic Location> VTI	M12119-02, MRUS,Velocity-Time Integral
<Vasculature Anatomic Location> HR	11948-7, LN, Fetal Heart Rate
<Vasculature Anatomic Location>	M12119-03, MRUS, Angle
<Vasculature Anatomic Location> VD	R-1025C, SRT, Vessel Intimal Diameter
<Vasculature Anatomic Location> VolFlow	M12119-06, MRUS, Vol Flow(TAMAX)
<Vasculature Anatomic Location> VolFlow.TAMEAN	M12119-07, MRUS,Vol Flow(TAMEAN)

Stomach	T-57000,SNM3,Stomach
Left Kidney	T-71000,SRT,Kidney
Right Kidney	T-71000,SRT,Kidney
Bladder	T-74000,SRT,Bladder
Gall Bladder	T-63000,SRT,Gall bladder
Liver	T-62000,SRT,Liver
Fetal Bowel	FG4031-03,MRUS,Fetal Bowel
Upper Extremities	FG4031-05,MRUS,Upper Extremities
Lower Extremities	FG4031-06,MRUS,Lower Extremities
Cardiac Activity	FG12239-01,MRUS,Cardiac Activity
4C HEART	FG4031-08,MRUS,4C HEART
Aorta	T-42000,SNM3,Aorta
Pulmonary Artery	T-44000,SNM3,Pulmonary Artery
ARCH	FG3010-01,MRUS,ARCH
Lateral Ventricles	FG4030-

							Echocardiography Left Ventricle
9	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-32500, $MeasType = DCID (12204) Echocardiography Right Ventricle
10	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-32300, $MeasType = DCID (12205) Echocardiography Left Atrium
11	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-32200, $MeasType = DCID (12206) Echocardiography Right Atrium
12	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-35400, $MeasType = DCID (12211) Echocardiography Aortic Valve
13	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-35300, $MeasType = DCID (12207) Echocardiography Mitral Valve
14	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject =

							EV (T-35200, $MeasType = DCID (12209) Echocardiography Pulmonic Valve
15	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-35100, Valv $MeasType = DCID (12208) Echocardiography Tricuspid Valve
16	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-42000, $MeasType= DCID (12212) Echocardiography Aorta
17	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-44000, $MeasType DCID (12210) = Echocardiography Pulmonary Artery
18	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-48600, $MeasType = DCID (12215) Echocardiography Vena Cavae
19	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-48581, Venous

							$MeasType = DCID (12214) Echocardiography Pulmonary Veins
20	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (P5-30031, $MeasType = DCID (12217) Echocardiography Cardiac Shunt
21	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (D4-30000, Anomaly of Cardiovascular $MeasType = DCID (12218) Echocardiography Congenital
22	>	CONTAINS	INCLUDE	DTID (5204) Wall Motion Analysis			
23	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (D3-90000, disease") $MeasType = DCID (90000) Pericardial disease
24	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (G-0394, $MeasType = DCID (12220) Echocardiography Common Measurements
25	>	CONTAINS	TEXT	(20121120,MRUS, "self-defined-measurementfile")			

1			CONTAINER	EV (121118, DCM,			
2	>	CONTAINS	NUM	EV (121033, DCM,		Units = DCID (7456) Units of Measure for Age	from Info
3	>	CONTAINS	CODE	EV (121032, DCM,		DCID (7455) Sex	from worklist or Info
4	>	CONTAINS	NUM	EV (8867-			from Info
5	>	CONTAINS	NUM	EV (F-008EC, SRT,			from Info
6	>	CONTAINS	NUM	EV (F-008ED, SRT, "Diastolic Blood Pressure")			from Info
7	>	CONTAINS	NUM	EV(18070-3,LN,"Right Atrium Systolic Pressure")			from Info
8	>	CONTAINS	NUM	EV (8302-			from worklist or Info
9	>	CONTAINS	NUM	EV (29463-			from worklist or Info
10	>	CONTAINS	NUM	EV (8277-			from Info
11	>>	INFERRED FROM	CODE	EV (8278-4, LN, "Body Surface Area Formula")		BCID (3663) Body Surface Area Equations	

B.4. TID (SELFTMP-2) Echo Procedure Summary Section

This is a private template referenced by TID(5200).

	NL	Rel with Parent	VT	Concept Name	Used in Modality	Value Set Constraint	Comment
1			CONTAINER	DT(12111,DCM,"Summary")			
2	>	CONTAINS	TEXT	EV(121106,DCM,"Comment")			from Info
3	>	CONTAINS	TEXT	(I12101-01,MRUS,"Primary Indications")			from Info
4	>	CONTAINS	TEXT	(I12101-02,MRUS,"Secondary Indications")			from Info

5	>	CONTAINS	TEXT	(I12101-03,MRUS,"CPT4 Code")			from Info
6	>	CONTAINS	TEXT	(I12101-04,MRUS,"CPT4 Description")			from Info
	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")			from report interface Comment
8	>	CONTAINS	TEXT	(I12101-05,MRUS,"Prompt")			from report interface Comment
9	>	CONTAINS	TEXT	(121071,DCM,"Findings")			from report interface Comment

B.5. TID (5202) ECHO SECTION

	NL	**Rel with Parent**	**VT**	**Concept Name**	**Used in MODALITY**	**Value Set Constraint**	**Comment**
1			CONTAINER	EV (121070,			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT,		$SectionSubject = EV (T-32600,	
3	>	CONTAINS	CONTAINER	DT (125007, DCM,			
4	>>	HAS CONCEPT MOD	CODE	EV (G-		BCID (12224) Ultrasound Image Modes	
5	>>	HAS CONCEPT MOD	CODE	DT			
6	>>	CONTAINS	INCLUDE	DTID (5203) Echo Measurement		$Measurement= $MeasType = DCID (12200) Echocardiography Left Ventricle $Method=CID (12227) Echocardiography	

	Measurement Method	

in TY	Value Set Constraint	Comment
	$Measurement = $Measurement $Method = $Method $TargetSite = BCID (12236) Echo Anatomic Sites $TargetSiteMod = BCID (12237) Echocardiography Anatomic Site Modifiers	
	This row is used only if the measurement or calculation this template is invoked with mandates it. Otherwise this row is not used. The values are taken from the BCID 12227	
	BCID (12221) Flow Direction	

DCID (12234) Respiration State

MRUS	M12201-02	Left ventricular Minor
MRUS	C12201-01	Mean Velocity of Circumferential Fiber Shortening
MRUS	M12201-03	A Distance
MRUS	M12201-04	B Distance
MRUS	M12201-05	Left ventricular internal diameter to BSA Ratio

B.9. CID (12202) Left Ventricle Volume

CSD	CV	Code Meaning
LN	18026-5	Left Ventricular End Diastolic Volume
LN	18148-7	Left Ventricular End Systolic Volume
LN	18043-0	Left Ventricular Ejection Fraction

B.10. CID (12203) Left Ventricle Other

CSD	CV	Code Meaning
LN	18087-7	Left Ventricle Mass
LN	18071-1	Left Ventricular Isovolumic Relaxation Time
SRT	G-037E	Left Ventricular Isovolumic Contraction Time
SRT	G-037F	Left Ventricular Index of Myocardial Performance
MRUS	M12203-01	Left Ventricle Pre-Ejection Period
MRUS	M12203-02	Left Ventricle Ejection Time
MRUS	C12203-01	Left ventricular Mass Weight Index
MRUS	C12203-02	Left Ventricle Pre-Ejection Period to Ejection Time Ratio

B.11. CID (12204) Echocardiography Right Ventricle

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
INCLUDE CID 12239 Cardiac Output Properties		
LN	20304-2	Right Ventricular Internal Diastolic Dimension
LN	20305-9	Right Ventricular Internal Systolic Dimension
SRT	G-0381	Right Ventricular Index of Myocardial Performance

CSD	CV	Code Meaning
MRUS	M12204-01	Right ventricular Major
MRUS	M12204-02	Right ventricular Minor
MRUS	M12204-03	Right ventricular Area at end-diastole
MRUS	M12204-04	Right ventricular Area at end-systole
MRUS	M12204-05	Right Ventricle Pre-Ejection Period
MRUS	M12204-06	Right Ventricle Ejection Time
MRUS	C12204-01	Right Ventricle Pre-Ejection Period to Ejection Time Ratio

B.12. CID (12205) Echocardiography Left Atrium

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	29469-4	Left Atrium Antero-posterior Systolic Dimension
LN	17985-3	Left Atrium to Aortic Root Ratio
LN	17977-0	Left Atrium Systolic Area
SRT	G-0383	Left Atrium Systolic Volume
MRUS	M12205-01	Left atrium Major
MRUS	M12205-02	Left atrium Minor
MRUS	C12205-01	Aortic Root to Left Atrium Ratio

B.13. CID (12206) Echocardiography Right Atrium

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	17988-7	Right Atrium Systolic Area
MRUS	M12206-01	Right atrium Major
MRUS	M12206-02	Right atrium Minor
MRUS	M12206-03	Right atrium Volume

B.14. CID (12207) Echocardiography Mitral Vaography yf03(o)4(g)4(r)-3(-4(

CSD	CV	Code Meaning

CSD	CV	Code Meaning
MRUS	M12207-25	Deceleration Time of Early diastolic velocity
MRUS	M12207-26	Deceleration Rate of Early diastolic velocity
MRUS	M12207-27	Mitral Stenosis Radius
MRUS	M12207-28	Mitral Stenosis Aliasing Velocity
MRUS	M12207-29	Mitral Stenosis Maximum Velocity
MRUS	M12207-30	Mitral Stenosis Area
MRUS	C12207-01	Mitral Stenosis Maximum Pressure Gradient

B.15. CID (12208) Echocardiography Tricuspid Valve

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
LN	18031-5	Tricuspid Valve E Wave Peak Velocity
LN	18030-7	Tricuspid Valve A Wave Peak Velocity
LN	18039-8	Tricuspid Valve E to A Ratio
SRT	G-0389	Tricuspid Valve Closure to Opening Time
MRUS	M12208-01	Tricuspid Valve E-Wave Duration
MRUS	M12208-02	Tricuspid Valve E Wave Pressure Gradient
MRUS	M12208-03	Tricuspid Valve A Wave Pressure Gradient
MRUS	M12207-35	MV E/Ea

B.16. CID (12209) Echocardiography Pulmonic Valve

INCLUDE CID 12220 Echocardiography Common Measurements
INCLUDE CID 12222 Orifice Flow Properties

B.17. CID (12210) Echocardiography Pulmonary Artery

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	18020-8	Main Pulmonary Artery Diameter

LN 18021-6/P <<

CSD	CV	Code Meaning
MRUS	M12214-03	Pulmonary Vein A-wave flow Velocity
MRUS	M12214-04	Pulmonary Vein Deceleration Time
MRUS	M12214-05	Pulmonary Vein Ratio of S-Wave velocity to D-wave velocity
MRUS	M12214-06	Pulmonary Vein Systolic fraction

B.21. CID (12215) Echocardiography Vena Cavae

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	18006-7	Inferior Vena Cava Diameter
MRUS	M12215-01	Superior Vena Cava Diameter

B.22. CID (12217) Echocardiography Cardiac Shunt

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12239 Cardiac Output Properties		
LN	29462-9	Pulmonary-to-Systemic Shunt Flow Ratio
MRUS	M12217-01	Pulmonary-sub-Systemic Shunt Flow Difference

B.23. CID (12218) Echocardiography Congenital

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
MRUS	M12218-01	Patent Ductus Arteriosus Diameter
MRUS	M12218-02	Patent Foramen Ovale Diameter
MRUS	M12218-03	Patent Ductus Arteriosus Diastolic Velocity
MRUS	M12218-04	Patent Ductus Arteriosus Systolic Velocity
MRUS	M12218-05	Coarctation of Pre-Ductus Velocity
MRUS	M12218-06	Coarctation of Post-Ductus Velocity
MRUS	M12218-07	Patent Ductus Arteriosus Diastolic Peak Gradient
MRUS	M12218-08	Patent Ductus Arteriosus Systolic Peak Gradient
MRUS	M12218-09	Coarctation of Pre-Ductus Peak Gradient
MRUS	M12218-10	Coarctation of Post-Ductus Peak Gradient

B.24. CID (12220) Echocardiography Common Measurements

CSD	CV	Code Meaning
LN	8867-4	Heart rate

B.25. CID (12221) Flow Direction

CSD	CV	Code Meaning
SRT	R-42047	Antegrade Flow
SRT	R-42E61	Regurgitant Flow

B.26. CID (12222) Orifice Flow Properties

CSD	CV	Code Meaning
SRT	G-038E	Cardiovascular Orifice Area
SRT	G-038F	Cardiovascular Orifice Diameter
SRT	G-0390	Regurgitant Fraction
LN	11726-7	Peak Velocity
LN	20352-1	Mean Velocity
LN	20247-3	Peak Gradient
LN	20256-4	Mean Gradient
LN	20354-7	Velocity Time Integral
LN	20168-1	Acceleration Time
LN	11653-3	End Diastolic Velocity
LN	20280-4	Pressure Half-Time
LN	20217-6	Deceleration Time
LN	33878-0	Volume Flow
LN	34141-2	Peak Instantaneous Flow Rate
LN	20216-8	Deceleration Slope
MRUS	M12222-05	Aliasing Velocity
MRUS	M12222-04	Time
MRUS	M12222-02	Acceleration Slope
MRUS	M12222-06	Flow Radius

CSD	CV	Code Meaning
MRUS	M12222-01	Angle
MRUS	M12222-08	Presure Gradient at end-Diastole
MRUS	M12222-07	Acceleration Time/Deceleration Time

B.27. CID (12224) Ultrasound Image Modes

CSD	CV	Code Meaning
SRT	G-03A2	2D mode
SRT	G-0394	M mode
SRT	R-409E2	Doppler Color Flow
SRT	G-0394	M mode
SRT	R-409E4	Doppler Pulsed
SRT	R-409E3	Doppler Continuous Wave
DCM	125230	Power Doppler
DCM	125231	3D mode
MRUS	IM12224-01	Tissue Doppler Imaging

B.28. CID (12226) Echocardiography Image View

CSD	CV	Code Meaning
SRT	G-A19B	Apical two chamber
SRT	G-A19C	Apical four chamber
SRT	G-0395	Apical long axis
SRT	G-0396	Parasternal long axis
SRT	G-0397	Parasternal short axis
SRT	G-0398	Parasternal short axis at the aortic valve level
SRT	G-0399	Parasternal short axis at the level of the mitral chords
SRT	G-039A	Parasternal short axis at the Mitral Valve level
SRT	G-039B	Parasternal short axis at the Papillary Muscle level
SRT	G-039C	Right Ventricular Inflow Tract View
SRT	G-039D	Right Ventricular Outflow Tract View
SRT	G-039E	Subcostal long axis
SRT	G-039F	Subcostal short axis
SRT	G-03A0	Suprasternal long axis
SRT	G-03A1	Suprasternal short axis

CSD

LVIDd Cube(M)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
LVIDd Teich(M)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
LVIDd LV Mass(Cube)(2D)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode;
LVIDd LV Mass(Cube)(M)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
LVIDd(BP Ellipse)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
LVIDd(M)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-0394,SRT,M Mode;
LVIDs(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode;
LVIDs Cube(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
LVIDs Teich(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
LVIDs Gibson(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
LVIDs Cube(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
LVIDs Teich(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
LVIDs Gibson(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
LVIDs(BP Ellipse)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
LVIDs(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode;
FS(Cube-M)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
FS(Teich-M)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
FS(Gibson-M)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
FS(Cube-2D)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method

IVSs(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode;
IVSs Teich(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
IVSs Teich(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
IVSs Cube(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
IVSs Cube(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
IVSs Gibson(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
IVSs Gibson(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
LVPW%(2D)	18053-9,LN,Left Ventricle Posterior Wall % Thickening	ImageMode = G-03A2,SRT,2D mode;
LVPW%(M)	18053-9,LN,Left Ventricle Posterior Wall % Thickening	ImageMode = G-0394,SRT,M Mode;
LVLd apical(Mod.Simpson)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
LVLd(A2C)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
LVLd(A4C)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVLd apical(SP Ellipse)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
LVLd apical(Bullet)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
LVLd apical(LV Mass A-L)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =125205,DCM,Area-Length Single Plane
LVLd2i	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane

LVLd4i	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
LVLs apical(Mod.Simpson)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode;
LVLs(A2C)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125226,DCM,Single Plane Ellipse
LVLs(A4C)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125226,DCM,Single Plane Ellipse
LVLs apical(SP Ellipse)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode;
LVLs apical(Bullet)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode;
LVLs2i	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
LVLs4i	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
LVPWs(2D)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode;
LVPWs(M)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode;
LVPWs Cube(2D)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
LVPWs Cube(M)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
LVPWs Teich(2D)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
LVPWs Teich(M)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
LVPWs Gibson(2D)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson

LVPWs Gibson(M)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
LVPWd(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode;
LVPWd(LV Mass-2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode;
LVPWd(LV Mass-M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
LVPWd(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode;
LVPWd Cube(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
LVPWd Cube(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
LVPWd Teich(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
LVPWd Teich(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
LVPWd Gibson(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
LVPWd Gibson(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
LV Major	M12201-01,MRUS,Left ventricular Major	ImageMode = G-03A2,SRT,2D mode;
LV Minor	M12201-02,MRUS,Left ventricular Minor	ImageMode = G-03A2,SRT,2D mode;
MVCF(Cube-M)	C12201-01,MRUS,Mean Velocity of Circumferential Fiber Shortening	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
MVCF(Teich-M)	C12201-01,MRUS,Mean Velocity of Circumferential Fiber Shortening	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
MVCF(Gibson-M)	C12201-01,MRUS,Mean Velocity of Circumferential Fiber Shortening	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
MVCF(Cube-2D)	C12201-01,MRUS,Mean Velocity of Circumferential Fiber Shortening	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
MVCF(Teich-2D)	C12201-01,MRUS,Mean Velocity of Circumferential Fiber Shortening	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
MVCF(Gibson-2D)	C12201-01,MRUS,Mean Velocity of Circumferential Fiber Shortening	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
a	M12201-03,MRUS,A Distance	ImageMode = G-03A2,SRT,2D mode;
d	M12201-04,MRUS,B Distance	ImageMode = G-03A2,SRT,2D mode;

LVIDd Index(M)	M12201-05,MRUS,Left ventricular internal diameter to BSA Ratio	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-0394,SRT,M Mode;
LVIDs Index(M)	M12201-05,MRUS,Left ventricular internal diameter to BSA Ratio	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-0394,SRT,M Mode;
LVIDd Index(2D)	M12201-05,MRUS,Left ventricular internal diameter to BSA Ratio	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-03A2,SRT,2D mode;
LVIDs Index(2D)	M12201-05,MRUS,Left ventricular internal diameter to BSA Ratio	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-03A2,SRT,2D mode;
rd2i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
rd4i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
rs2i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
rs4i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
LV Area(s)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode = G-03A2,SRT,2D mode;
LVAs apical(SP Ellipse)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode = G-03A2,SRT,2D mode; ImageView = G-0395,SRT,Apical long axis;
LVAs sax MV(Mod.Simpson)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level;
LVAs sax PM	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level;
LVAs(A2C)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane

LVAs(A4C)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAs sax MV(BP Ellipse)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =125211,DCM,Biplane Ellipse
LVAs sax MV(Bullet)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =VM12228-01,MRUS,Bullet
LVAs apical(BP Ellipse)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
LV Area(d)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode;
LVAd apical(SP Ellipse)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-0395,SRT,Apical long axis;
LVAd sax MV(Mod.Simpson)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level;
LVAd sax PM	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level;
LVAd(A2C)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAd(A4C)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAd sax MV(BP Ellipse)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =125211,DCM,Biplane Ellipse
LVAd sax MV(Bullet)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =VM12228-01,MRUS,Bullet

LVAd apical(BP Ellipse)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-0395,SRT,Apical long axis; Method =125211,DCM,Biplane Ellipse
LVAd sax Epi(LV Mass T-E)	G-0379,SRT,Left Ventricle Epicardial Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LVAd sax Epi(LV Mass A-L)	G-0379,SRT,Left Ventricle Epicardial Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125205,DCM,Area-Length Single Plane
LVAd sax Endo(LV Mass T-E)	M12240-01,MRUS,Left Ventricle Endocardiac Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LVAd sax Endo(LV Mass A-L)	M12240-01,MRUS,Left Ventricle Endocardiac Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125205,DCM,Area-Length Single Plane
EDV(SP Ellipse)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
EDV(BP Ellipse)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
EDV(Bullet)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
EDV(Mod.Simpson)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
EDV(Simp SP-A2C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
EDV(Simpson BP)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
EDV(Simp BP-A2C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane

EDV(Simp BP-A4C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
EDV(Cube-M)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
EDV(Teich-M)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
EDV(Gibson-M)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
EDV(Cube-2D)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
EDV(Teich-2D)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
EDV(Gibson-2D)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
EDV(Simp SP-A4C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
ESV(SP Ellipse)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
ESV(BP Ellipse)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
ESV(Bullet)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
ESV(Mod.Simpson)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
ESV(Simp SP-A2C)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
ESV(Simpson BP)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
ESV(Simp BP-A2C)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane

ESV(Simp BP-A4C)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
ESV(Cube-M)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
ESV(Teich-M)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
ESV(Gibson-M)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
ESV(Cube-2D)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
ESV(Teich-2D)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
ESV(Gibson-2D)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
ESV(Simp SP-A4C)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
EF(SP Ellipse)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
EF(BP Ellipse)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
EF(Bullet)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
EF(Mod.Simpson)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
EF(A2C)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
EF(Simpson BP)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
EF2(Simpson BP)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane

EF4(Simpson BP)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
EF(Cube-M)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
EF(Teich-M)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
EF(Gibson-M)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
EF(Cube-2D)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
EF(Teich-2D)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
EF(Gibson-2D)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
EF(A4C)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVOT Area	G-038E,SRT,Cardiovascular Orifice Area	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(2D)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(M)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-0394,SRT,M Mode;
LVOT Diam(MVA VTI)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(AVA VTI)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(AVA Vmax)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Vmax	11726-7,LN,Peak Velocity	
LVOT Vmax(LVOT VTI)	11726-7,LN,Peak Velocity	
LVOT Vmean	20352-1,LN,Mean Velocity	
LVOT PGmax	20247-3,LN,Peak Gradient	
LVOT PGmax(LVOT VTI)	20247-3,LN,Peak Gradient	
LVOT PGmean	20256-4,LN,Mean Gradient	

LVOT VTI	20354-7,LN,Velocity Time Integral	
LVOT VTI(MVA VTI)	20354-7,LN,Velocity Time Integral	
LVOT VTI(AVA VTI)	20354-7,LN,Velocity Time Integral	
LVOT AccT	20168-1,LN,Acceleration Time	
LVOT	M12222-01,MRUS, Angle	
LVOT Acc Slope	M12222-02,MRUS, Acceleration Slope	
LV Mass(Cube-M)	18087-7,LN,Left Ventricle Mass	ImageMode =G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
LV Mass(T-E)	18087-7,LN,Left Ventricle Mass	ImageMode =G-03A2,SRT,2D mode; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LV Mass(A-L)	18087-7,LN,Left Ventricle Mass	ImageMode =G-03A2,SRT,2D mode; Method =125205,DCM,Area-Length Single Plane
LV Mass(Cube-2D)	18087-7,LN,Left Ventricle Mass	ImageMode =G-03A2,SRT,2D mode;
IVRT	18071-1,LN,Left Ventricular Isovolumic Relaxation Time	
IVCT	G-037E,SRT,Left Ventricular Isovolumic Contraction Time	
LVIMP(M)	G-037F,SRT,Left Ventricular Index of Myocardial Performance	ImageMode =G-0394,SRT,M Mode;
LVIMP(Doppler)	G-037F,SRT,Left Ventricular Index of Myocardial Performance	

LV Mass-I(Cube-M)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
LV Mass-I(T-E)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-03A2,SRT,2D mode; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LV Mass-I(A-L)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-03A2,SRT,2D mode; Method =125205,DCM,Area-Length Single Plane
LV Mass-I(Cube-2D)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-03A2,SRT,2D mode;
LVPEP/ET(M)	C12203-02,MRUS,Left Ventricle Pre-Ejection Period to Ejection Time Ratio	ImageMode =G-0394,SRT,M Mode;
LVPEP/ET(Doppler)	C12203-02,MRUS,Left Ventricle Pre-Ejection Period to Ejection Time Ratio	
LVOT SV	F-32120,SRT,Stroke Volume	
SV(SP Ellipse)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
SV(BP Ellipse)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
SV(Bullet)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
SV(Mod.Simpson)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
SV(A2C)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
SV(Simpson BP)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
SV2(Simpson BP)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
SV4(Simpson BP)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane

CO(Cube-M)	F-32100,SRT,Cardiac Output	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
CO(Teich-M)	F-32100,SRT,Cardiac Output	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
CO(Gibson-M)	F-32100,SRT,Cardiac Output	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
CO(Cube-2D)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
CO(Teich-2D)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
CO(Gibson-2D)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
CO(A4C)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVOT CI	F-32110,SRT,Cardiac Index	
CI(SP Ellipse)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
CI(BP Ellipse)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
CI(Bullet)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
CI(Mod.Simpson)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
CI(A2C)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
CI(Simpson BP)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
CI2(Simpson BP)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
CI4(Simpson BP)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane

CI(Cube-M)	F-32110,SRT,Cardiac Index	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
CI(Teich-M)	F-32110,SRT,Cardiac Index	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
CI(Gibson-M)	F-32110,SRT,Cardiac Index	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
CI(Cube-2D)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
CI(Teich-2D)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
CI(Gibson-2D)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
CI(A4C)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVOT SI	F-00078,SRT,Stroke Index	
SI(SP Ellipse)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
SI(BP Ellipse)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
SI(Bullet)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
SI(Mod.Simpson)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
SI(A2C)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
SI(Simpson BP)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
SI2(Simpson BP)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
SI4(Simpson BP)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane

SI(Cube-M)	F-00078,SRT,Stroke Index	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
SI(Teich-M)	F-00078,SRT,Stroke Index	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
SI(Gibson-M)	F-00078,SRT,Stroke Index	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
SI(Cube-2D)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
SI(Teich-2D)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
SI(Gibson-2D)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
SI(A4C)	F-00078,SRT,Stroke Index	G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane

B.40.2. Right Ventricle Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
RVDd(2D)	20304-2,LN,Right Ventricular Internal Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode;
RVDd(M)	20304-2,LN,Right Ventricular Internal Diastolic Dimension	ImageMode = G-0394,SRT,M Mode;
RVDs(2D)	20305-9,LN,Right Ventricular Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode;
RVDs(M)	20305-9,LN,Right Ventricular Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode;
RVIMP	G-0381,SRT,Right Ventricular Index of Myocardial Performance	
RVSP	G-0380,SRT,Right Ventricular Peak Systolic Pressure	
RVAWd(2D)	18153-7,LN,Right Ventricular Anterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode;
RVAWd(M)	18153-7,LN,Right Ventricular Anterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode;
RVAWs(2D)	18157-8,LN,Right Ventricular Anterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode;
RVAWs(M)	18157-8,LN,Right Ventricular Anterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode;
RV Major	M12204-01,MRUS,Right ventricular Major	ImageMode = G-03A2,SRT,2D mode;

RV Minor	M12204-02,MRUS,Right ventricular Minor	ImageMode = G-03A2,SRT,2D mode;
RV Area(d)	M12204-03,MRUS,Right ventricular Area at end-diastole	ImageMode = G-03A2,SRT,2D mode;
RV Area(s)	M12204-04,MRUS,Right ventricular Area at end-systole	ImageMode = G-03A2,SRT,2D mode;
RVPEP(M)	M12204-05,MRUS,Right Ventricle Pre-Ejection Period	ImageMode = G-0394,SRT,M Mode;
RVPEP(Doppler)	M12204-05,MRUS,Right Ventricle Pre-Ejection Period	
RVET(M)	M12204-06,MRUS,Right Ventricle Ejection Time	ImageMode = G-0394,SRT,M Mode;
RVET(RVIMP)	M12204-06,MRUS,Right Ventricle Ejection Time	
RVET(Doppler)	M12204-06,MRUS,Right Ventricle Ejection Time	
RVPEP/ET(M)	C12204-01,MRUS,Right Ventricle Pre-Ejection Period to Ejection Time Ratio	ImageMode = G-0394,SRT,M Mode;
RVPEP/ET(Doppler)	C12204-01,MRUS,Right Ventricle Pre-Ejection Period to Ejection Time Ratio	
RVOT HR	8867-4,LN,Heart rate	
RVOT Diam(2D)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode = G-03A2,SRT,2D mode;
RVOT Diam(M)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode = G-0394,SRT,M Mode;
RVOT Vmax	11726-7,LN,Peak Velocity	
RVOT Vmax(RVOT VTI)	11726-7,LN,Peak Velocity	
RVOT Vmean	20352-1,LN,Mean Velocity	
RVOT PGmax	20247-3,LN,Peak Gradient	
RVOT PGmax(RVOT VTI)	20247-3,LN,Peak Gradient	
RVOT PGmean	20256-4,LN,Mean Gradient	
RVOT VTI	20354-7,LN,Velocity Time Integral	
RVOT	M12222-01,MRUS,Angle	

B.40.3. Left Atrium Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
LA Diam(2D)	29469-4,LN,Left Atrium Antero-posterior Systolic Dimension	ImageMode = G-03A2,SRT,2D mode;
LA Diam(M)	29469-4,LN,Left Atrium Antero-posterior Systolic Dimension	ImageMode = G-0394,SRT,M Mode;

LA Diam(LA Vol A-L)	29469-4,LN,Left Atrium Antero-posterior Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method = 125205,DCM,Area-Length Single Plane
LA Diam(LA/Ao-2D)	29469-4,LN,Left Atrium Antero-posterior Systolic Dimension	ImageMode = G-03A2,SRT,2D mode;
LA Diam(LA/Ao-M)	29469-4,LN,Left Atrium Antero-posterior Systolic Dimension	ImageMode = G-0394,SRT,M Mode;
LA/Ao(2D)	17985-3,LN,Left Atrium to Aortic Root Ratio	ImageMode = G-03A2,SRT,2D mode;
LA/Ao(M)	17985-3,LN,Left Atrium to Aortic Root Ratio	ImageMode = G-0394,SRT,M Mode;
LA Area	17977-0,LN,Left Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode;
LAA(A2C)	17977-0,LN,Left Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method = 125205,DCM,Area-Length Single Plane
LAA(A4C)	17977-0,LN,Left Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method = 125205,DCM,Area-Length Single Plane
LA Vol(A-L)	G-0383,SRT,Left Atrium Systolic Volume	ImageMode = G-03A2,SRT,2D mode; Method = 125205,DCM,Area-Length Single Plane
LA Vol(A2C)	G-0383,SRT,Left Atrium Systolic Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method = 125208,DCM,Method of Disks, Single Plane
LA Vol(A4C)	G-0383,SRT,Left Atrium Systolic Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method = 125208,DCM,Method of Disks, Single Plane
LA Major	M12205-01,MRUS,Left atrium Major	ImageMode = G-03A2,SRT,2D mode;
LA Minor	M12205-02,MRUS,Left atrium Minor	ImageMode = G-03A2,SRT,2D mode;
LeftA.AR/LA.M	C12205-01,MRUS,Aortic Root to Left Atrium Ratio	

B.40.4. Right Atrium Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*

RAP	18070-3,LN,Right Atrium Systolic Pressure	
RA Area	17988-7,LN,Right Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode;
RA Major	M12206-01,MRUS,Right atrium Major	ImageMode = G-03A2,SRT,2D mode;
RA Minor	M12206-02,MRUS,Right atrium Minor	ImageMode = G-03A2,SRT,2D mode;
RA Vol(A4C)	M12206-03,MRUS,Right atrium Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method = 125208,DCM,Method of Disks, Single Plane

B.40.5. Aortic Valve Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
ACS(2D)	17996-0,LN,Aortic Valve Cusp Separation	ImageMode = G-03A2,SRT,2D mode;
ACS(M)	17996-0,LN,Aortic Valve Cusp Separation	ImageMode = G-0394,SRT,M Mode;
AV AccT/ET	G-0382,SRT,Ratio of Aortic Valve Acceleration Time to Ejection Time	
AV HR	8867-4,LN,Heart rate	

AR Ved	11653-3,LN,End Diastolic Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow
AV Vmax	11726-7,LN,Peak Velocity	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Vmax	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR Vmax(AR VTI)	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR Vmax(AR PHT)	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR Vmax(PISA AR)	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AV Vmax(AV VTI)	11726-7,LN,Peak Velocity	Flow Direction = R-42047,SRT,Antegrade Flow;
AV Vmean	20352-1,LN,Mean Velocity	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Vmean	20352-1,LN,Mean Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV PGmax	20247-3,LN,Peak Gradient	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PGmax	20247-3,LN,Peak Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV PGmax(AV VTI)	20247-3,LN,Peak Gradient	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PGmax(AR VTI)	20247-3,LN,Peak Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR PGmax(AR PHT)	20247-3,LN,Peak Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV PGmean	20256-4,LN,Mean Gradient	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PGmean	20256-4,LN,Mean Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV VTI	20354-7,LN,Velocity Time Integral	Flow Direction = R-42047,SRT,Antegrade Flow;
AR VTI	20354-7,LN,Velocity Time Integral	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV VTI(Qp/Qs)	20354-7,LN,Velocity Time Integral	Flow Direction = R-42047,SRT,Antegrade Flow;
AR VTI(PISA AR)	20354-7,LN,Velocity Time Integral	Flow Direction = R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AV VTI(AVA VTI)	20354-7,LN,Velocity Time Integral	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PHT	20280-4,LN,Pressure Half-Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV AccT	20168-1,LN,Acceleration Time	Flow Direction = R-42047,SRT,Antegrade Flow;
AV DecT	20217-6,LN,Deceleration Time	Flow Direction = R-42047,SRT,Antegrade Flow;
AR DcT	20217-6,LN,Deceleration Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR DecT	20217-6,LN,Deceleration Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV Acc Slope	M12222-02,MRUS,Acceleration Slope	Flow Direction = R-42047,SRT,Antegrade Flow;

AR Rad	M12222-06,MRUS,Flow Radius	Flow Direction = R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
AR Als.Vel	M12222-05,MRUS,Aliasing Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
AR Time	M12222-04,MRUS,Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR DcR	M12222-03,MRUS,Deceleration Rate	Flow Direction = R-42E61,SRT,Regurgitant Flow;

MV C-O dur(M)	G-0387,SRT,Mitral Valve Closure to Opening Time	ImageMode = G-0394,SRT,M Mode ;
MV C-O dur(Doppler)	G-0387,SRT,Mitral Valve Closure to Opening Time	
dP/dt	18035-6,LN,Mitral Regurgitation Dp/dt derived from Mitral Reg. velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MCS(2D)	M12207-01,MRUS,Mitral valve cusp separate distance	ImageMode = G-03A2,SRT,2D mode ;
MCS(M)	M12207-01,MRUS,Mitral valve cusp separate distance	ImageMode = G-0394,SRT,M Mode ;
MV D-E Slope	M12207-02,MRUS,Mitral Valve D-E Slope	ImageMode = G-0394,SRT,M Mode ;
MV A Amp	M12207-03,MRUS,Amplitude of the A wave	ImageMode = G-0394,SRT,M Mode ;
MV E Amp	M12207-04,MRUS,Amplitude of the E wave	ImageMode = G-0394,SRT,M Mode ;
MV DE	M12207-05,MRUS,Amplitude from D Point to E Point	ImageMode = G-0394,SRT,M Mode ;
MV E PG	M12207-06,MRUS,Mitral Valve E-wave Pressure Gradient	
MV A PG	M12207-07,MRUS,Mitral Valve A-wave Pressure Gradient	
MV E VTI	M12207-08,MRUS,E wave Velocity Time Integral	Flow Direction =R-42047,SRT,Antegrade Flow;
MV A VTI	M12207-09,MRUS,A wave Velocity Time Integral	Flow Direction =R-42047,SRT,Antegrade Flow;
MV E Dur	M12207-10,MRUS,Mitral Valve E-Wave Duration	
Sa(medial)	M12207-11,MRUS,Systolic Velocity of the Mitral Annulus(medial)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea(medial)	M12207-12,MRUS,Early diastolic velocity of the mitral annulus(medial)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Aa(medial)	M12207-13,MRUS,Late diastolic velocity of the mitral annulus(medial)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea/Aa(medial)	M12207-14,MRUS,Early diastolic velocity to Late diastolic velocity Ratio	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ata(medial)	M12207-15,MRUS,Acceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ara(medial)	M12207-16,MRUS,Acceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;

Dta(medial)	M12207-17,MRUS,Deceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dra(medial)	M12207-18,MRUS,Deceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Sa(lateral)	M12207-19,MRUS,Systolic Velocity of the Mitral Annulus(lateral)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea(lateral)	M12207-20,MRUS,Early diastolic velocity of the mitral annulus(lateral)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Aa(lateral)	M12207-21,MRUS,Late diastolic velocity of the mitral annulus(lateral)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea/Aa(lateral)	M12207-22,MRUS,Early diastolic velocity to Late diastolic velocity Ratio	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ata(lateral)	M12207-23,MRUS,Acceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ara(lateral)	M12207-24,MRUS,Acceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dta(lateral)	M12207-25,MRUS,Deceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dra(lateral)	M12207-26,MRUS,Deceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
MS Rad	M12207-27,MRUS,Mitral Stenosis Radius	ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MS Als.Vel	M12207-28,MRUS,Mitral Stenosis Aliasing Velocity	ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MS Vmax	M12207-29,MRUS,Mitral Stenosis Maximum Velocity	
MS Vmax(PISA MS)	M12207-29,MRUS,Mitral Stenosis Maximum Velocity	Method = 125216,DCM,Proximal Isovelocity Surface Area

MV Acc Slope	M12222-02,MRUS,Acceleration Slope	Flow Direction =R-42047,SRT, Antegrade Flow;
dt	M12222-04,MRUS,Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MR Rad	M12222-06,MRUS,Flow Radius	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
MR Als.Vel	M12222-05,MRUS,Aliasing Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
MV	M12222-01,MRUS,Angle	Flow Direction =R-42047,SRT,Antegrade Flow;
MR	M12222-01,MRUS,Angle	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MV SV	F-32120,SRT,Stroke Volume	
MV CO	F-32100,SRT,Cardiac Output	
MV CI	F-32110,SRT,Cardiac Index	
MV SI	F-00078,SRT,Stroke Index	
E/Ea	M12207-35,MRUS,MV E/Ea	
PISA	M12222-09,MRUS, Effective Regurgitant Orifice Area	

B.40.7. Pulmonic Valve Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
PV	M12222-01,MRUS,Angle	Flow Direction =R-42047,SRT,Antegrade Flow;
PR	M12222-01,MRUS,Angle	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV HR	8867-4,LN,Heart rate	
PR Flow	33878-0,LN,Volume Flow	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
PR Flow Rate	34141-2,LN,Peak Instantaneous Flow Rate	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
PV Diam	G-038F,SRT,Cardiovascular Orifice Diameter	Flow Direction =R-42047,SRT,Antegrade Flow; ImageMode = G-03A2,SRT,2D mode;

PR PGed	M12222-08,MRUS,Presure Gradient at end-Diastole	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR PGed(PAEDP)	M12222-08,MRUS,Presure Gradient at end-Diastole	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV SV	F-32120,SRT,Stroke Volume	
PV CO	F-32100,SRT,Cardiac Output	
PV CI	F-32110,SRT,Cardiac Index	
PV SI	F-00078,SRT,Stroke Index	
PISA	M12222-09,MRUS, Effective Regurgitant Orifice Area	

B.40.8. Tricuspid Valve Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
TV E Vel	18031-5,LN,Tricuspid Valve E Wave Peak Velocity	
TV E Vel(TV E/A)	18031-5,LN,Tricuspid Valve E Wave Peak Velocity	
TV A Vel	18030-7,LN,Tricuspid Valve A Wave Peak Velocity	
TV A Vel(TV E/A)	18030-7,LN,Tricuspid Valve A Wave Peak Velocity	
TV E/A	18039-8,LN,Tricuspid Valve E to A Ratio	
TV E/A(TV E/A)	18039-8,LN,Tricuspid Valve E to A Ratio	
TV C-O dur	G-0389,SRT,Tricuspid Valve Closure to Opening Time	
TV	M12222-01,MRUS,Angle	Flow Direction =R-42047,SRT,Antegrade Flow;
TR	M12222-01,MRUS,Angle	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV HR	8867-4,LN,Heart rate	
TR Flow	33878-0,LN,Volume Flow	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TR Flow Rate	34141-2,LN,Peak Instantaneous Flow Rate	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area

TVA	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT, Antegrade Flow; ImageMode = G-03A2,SRT,2D mode; Method = 125220,DCM,Planimetry
TVA(PHT)	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT, Antegrade Flow; Method = 125210,DCM,Area by Pressure Half-Time
TV Diam	G-038F,SRT,Cardiovascular Orifice Diameter	Flow Direction =R-42047,SRT, Antegrade Flow; ImageMode = G-03A2,SRT,2D mode;
TR Fraction	G-0390,SRT,Regurgitant Fraction	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TV Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV Vmax(TV PHT)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TV Vmax(TV VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Vmax(TR VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR Vmax(PISA TR)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TR Vmax(RVSP)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV PGmax(TV PHT)	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TV PGmax(TV VTI)	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TV PGmax	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TR PGmax	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR PGmax(TR VTI)	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR PGmax(RVSP)	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV PGmean	20256-4,LN,Mean Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TR PGmean	20256-4,LN,Mean Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42047,SRT, Antegrade Flow;
TR VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR VTI(PISA TR)	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
TV PHT	20280-4,LN,Pressure Half-Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV AccT	20168-1,LN,Acceleration Time	Flow Direction =R-42047,SRT, Antegrade Flow;

Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
Slope	Flow Direction =R-42E61,SRT,Regurgitant Flow;
pid	Flow Direction =R-42047,SRT, Antegrade Flow;
pid ressure	Flow Direction =R-42047,SRT, Antegrade Flow;
pid ressure	Flow Direction =R-42047,SRT, Antegrade Flow;
eration	Flow Direction =R-42047,SRT, Antegrade Flow;
eration	Flow Direction =R-42047,SRT, Antegrade Flow;
Radius	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
ng	ImageMode = R-409E2, SRT, Doppler Color Flow;
me	
put	
e	
fective	

AC q95.ET1 34664 488.23 89.184 34.2 reW*n236 (e

rements

Ao Desc Diam(2D)	18013-3,LN,Descending Aortic Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Desc Diam(M)	18013-3,LN,Descending Aortic Diameter	ImageMode = G-0394,SRT,M Mode;
Ao st junct(2D)	M12212-01,MRUS,Aortic Sinotubular junction Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao st junct(M)	M12212-01,MRUS,Aortic Sinotubular junction Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Sinus Diam(2D)	M12212-02,MRUS,Aortic Sinus Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Sinus Diam(M)	M12212-02,MRUS,Aortic Sinus Diameter	ImageMode = G-0394,SRT,M Mode;
Duct Art Diam	M12212-03,MRUS,Ductus Artery Diameter	ImageMode = G-03A2,SRT,2D mode;
Pre Ductal	M12212-04,MRUS,Previous Ductal Diameter	ImageMode = G-03A2,SRT,2D mode;
LCA	M12212-05,MRUS,Left Coronary Artery Diameter	ImageMode = G-03A2,SRT,2D mode;
RCA	M12212-06,MRUS,Right Coronary Artery Diameter	ImageMode = G-03A2,SRT,2D mode;
AAo Vmax	11726-7,LN,Peak Velocity	
DAo Vmax	11726-7,LN,Peak Velocity	
AAo PGmax	20247-3,LN,Peak Gradient	
DAo PGmax	20247-3,LN,Peak Gradient	

B.40.10. Pulmonary Artery Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
MPA Diam(2D)	18020-8,LN,Main Pulmonary Artery Diameter	ImageMode =G-03A2,SRT,2D mode;
MPA Diam(M)	18020-8,LN,Main Pulmonary Artery Diameter	ImageMode =G-0394,SRT,M Mode;
RPA Diam(2D)	18021-6,LN,Right Pulmonary Artery Diameter	ImageMode =G-03A2,SRT,2D mode;
RPA Diam(M)	18021-6,LN,Right Pulmonary Artery Diameter	ImageMode =G-0394,SRT,M Mode;
LPA Diam(2D)	18019-0,LN,Left Pulmonary Artery Diameter	ImageMode =G-03A2,SRT,2D mode;
LPA Diam(M)	18019-0,LN,Left Pulmonary Artery Diameter	ImageMode =G-0394,SRT,M Mode;
MPA Vmax	G-038A,SRT,Main Pulmonary Artery Peak Velocity	
Post Ductal	M12210-01,MRUS,Posterior ductal Diameter	ImageMode =G-03A2,SRT,2D mode;
PAEDP	C12210-01,MRUS,Pulmonary Artery End Diastolic Pressure	
LPA Vmax	11726-7,LN,Peak Velocity	
RPA Vmax	11726-7,LN,Peak Velocity	
MPA PGmax	20247-3,LN,Peak Gradient	
LPA PGmax	20247-3,LN,Peak Gradient	
RPA PGmax	20247-3,LN,Peak Gradient	

B.40.11. Vena Cava Measurements lQ711.5 11 316 8.04yena CtyC1800

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
IVC Diam(Insp)	18006-7,LN,Inferior Vena Cava Diameter	RespiratoryCyclePoint=F-20010,SRT, During Inspiration; ImageMode =G-03A2,SRT,2D mode;
IVC Diam(Expir)	18006-7,LN,Inferior Vena Cava Diameter	RespiratoryCyclePoint=F-20030,SRT, During Expiration70.63 632.14 Tm0 g[

Q EMC[365.59 611.5 03 7[Q711.5 11 316 8.

2808/6P#057C<d EMC /u5 664 61f1 0 0 1 316 51 647 74 898m0 cl \]TJ11TO898mQ EMC c3

PVein D Vel	M12214-02,MRUS,Pulmonary Vein D-wave flow Velocity	
PVein A Vel	M12214-03,MRUS,Pulmonary Vein A-wave flow Velocity	
PVein DecT	M12214-04,MRUS,Pulmonary Vein Deceleration Time	
PVein S/D	M12214-05,MRUS,Pulmonary Vein Ratio of S-Wave velocity to D-wave velocity	
PVein SF	M12214-06,MRUS,Pulmonary Vein Systolic fraction	

B.40.13. Cardiac Shunt Study Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
Qp/Qs	29462-9,LN,Pulmonary-to-Systemic Shunt Flow Ratio	

Coarc Pre-Duct PG	M12218-09,MRUS,Coarctation of Pre-Ductus Pressure Gradient	
Coarc Post-Duc PG	M12218-10,MRUS,Coarctation of Post-Ductus Pressure Gradient	
VSD Diam	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
ASD Diam	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
VSD Vmax	11726-7,LN,Peak Velocity	
ASD Vmax	11726-7,LN,Peak Velocity	
VSD PGmax	20247-3,LN,Peak Gradient	
ASD PGmax	20247-3,LN,Peak Gradient	

B.40.15. Pericardial Disease Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
PEd(2D)	C90000-01,MRUS,Pericard Effusion at end-diastole	ImageMode =G-03A2,SRT,2D mode;
PEd(M)	C90000-01,MRUS,Pericard Effusion at end-diastole	ImageMode =G-0394,SRT,M Mode;
PEs(2D)	C90000-02,MRUS,Pericard Effusion at end-systole	ImageMode =G-03A2,SRT,2D mode;
PEs(M)	C90000-02,MRUS,Pericard Effusion at end-systole	ImageMode =G-0394,SRT,M Mode;

B.40.16. Heart Rate Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
HR	8867-4 LN Heart rate	Image Mode = G-0394,SRT,M Mode

C. Appendix : Vascular structured reporting template

This appendix lists the DICOM Structured Report (SR) mappings used in the Vascular Structured Reports of ultrasound system SR files.

The mappings are organized in a manner similar to the DICOM SR Templates as described in PS 3.16 of the DICOM Standard. The Vascular Report mappings follow the DICOM SR Template TID 5100: Vascular Ultrasound Procedure Report, except where noted.

All private code values use the Coding Scheme Designator "MRUS".

C.1. TID (5100) Vascular Ultrasoud Report

This is the template for the root the content tree for the vascular ultrasound procedure report.

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1			CONTAINER	EV (125100, DCM,			
2	>	HAS OBS CONTEXT	CODE	EV (R-40FB8, SRT,		DCID (12102) Temporal Periods Relating To Procedure or Therapy	
3	>	HAS CONCEPT MOD	INCL UDE	DTID (1204) Language of Content Item and Descendants			
4	>	HAS OBS CONTEXT	INCLUDE	DTID (1001) Observation Context			
5	>	CONTAINS	INCLUDE	DTID (5101) Vascular Patient Characteristics			
6	>	CONTAINS	CONTAINER	EV (111028, DCM,			

9	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12105) Intracranial Cerebral Vessels	
10	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12105) Intracranial Cerebral Vessels	
11	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-40501, $SectionLaterality = EV (G-A103, $Anatomy = DCID (12106) Intracranial Cerebral Vessels (unilateral)	
12	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12104) Extracranial Arteries $AnatomyRatio = DCID (12123) Carotid Ratios	

13	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12104) Extracranial Arteries $AnatomyRatio = DCID (12123) Carotid Ratios	
14	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12109) Lower Extremity Arteries $AnatomyRatio = 8581-1,LN,Tibial/brachial index	
15	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-470 $SectionLaterality = EV (G- $Anatomy = DCID (12109) Lower Extremity Arteries $AnatomyRatio = 8581-1,LN,Tibial/brachial index	
16	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12110) Lower Extremity Veins	

17	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-of $SectionLaterality = EV (G-$Anatomy = DCID (12110) Lower Extremity Veins	
18	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-$SectionLaterality = EV (G-$Anatomy = DCID (12107) Upper Extremity Arteries	
19	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-$SectionLaterality = EV (G-$Anatomy = DCID (12107) Upper Extremity Arteries	
20	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-$SectionLaterality = EV (G-$Anatomy = DCID (SELFCID-2) Upper Extremity Arteries(unilateral)	

21	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12108) Upper Extremity Veins	
22	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12108) Upper Extremity Veins	
23	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12111) Abdominal Arteries (lateral)	
24	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12111) Abdominal Arteries (lateral)	

25	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-46002, SR $SectionLaterality = EV (G-A103, $Anatomy = DCID (12112) Abdominal Arteries (unilateral)	
26	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12113) Abdominal Veins (lateral)	
27	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12113) Abdominal Veins (lateral)	
28	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G-A103, $Anatomy = DCID (12114) Abdominal Veins (unilateral)	

29	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-71019, $SectionLaterality = EV (G- $Anatomy = DCID (12115) Renal Vessels	
30	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-71019, $SectionLaterality = EV (G- $Anatomy = DCID (12115) Renal Vessels	
31	>	CONTAINS	INCLUDE	DTID (5105) Ultrasound Graft Section			
32	>	CONTAINS	TEXT	(20121120,MRUS, "self-defined-measurementfile")			

C.2. TID (1001) Observation Context

This template specifies attributes of observation context that may be defined, extended or replaced at any location in the SR tree.

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1	>	HAS OBS CONTEXT	CODE	EV (121005,DCM,		(121006,DCM,	
2	>	HAS OBS CONTEXT	PNAME	EV (121008,DCM,		Operator from Info	
3	>	HAS OBS CONTEXT	TEXT	EV (121009,DCM,		Institution Name (0008,0080) of the General Equipment Module	

4	>	HAS OBS CONTEXT	CODE	EV (121010,DCM, Role in the		(121093, DCM, "Sonographer")	
5	>	HAS OBS CONTEXT	CODE	EV (121024, DCM,		(121025, DCM,	
6	>	HAS OBS CONTEXT	PNAME	EV (121029,DCM,		(0010,0010) in Patient Module	
7	>	HAS OBS CONTEXT	DATE	EV (121031,DCM,		Date (0010,0030) in Patient Module	
8	>	HAS OBS CONTEXT	CODE	EV (121032,DCM,		value equivalent to (0010,0040) in Patient Module	
9	>	HAS OBS CONTEXT	NUM	EV (121033,DCM,		(0010,1010) in Patient Study Module	

C.3. TID (5101) Vascular Patient Characteristics

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1			CONTAINER	EV (121118, DCM,			
2	>	CONTAINS	NUM	EV (121033, DCM,		Units = DCID (7456) Units of Measure for Age	
3	>	CONTAINS	CODE	EV (121032, DCM,		DCID (7455) Sex	
4	>	CONTAINS	NUM	EV (8867-			
5	>	CONTAINS	NUM	EV (F-008EC, SRT,			

6	>	CONTAINS	NUM	EV (F-008ED, SRT, "Diastolic Blood Pressure")			

C.4. TID (5102) Vascular Procedure Summary Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	COMMENT
1			CONTAINER	DT (121111, DCM,			
2	>	CONTAINS	TEXT	DCID (12101) Vascular Summary			from Info comment
3	>	CONTAINS	TEXT	(I12101-01,MRUS,"Primary Indications")			from Info
4	>	CONTAINS	TEXT	(I12101-02,MRUS,"Secondary Indications")			from Info
5	>	CONTAINS	TEXT	(I12101-03,MRUS,"CPT4 Code")			from Info
6	>	CONTAINS	TEXT	(I12101-04,MRUS,"CPT4 Description")			from Info
7	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")			From report interface Comment
8	>	CONTAINS	TEXT	(I12101-05,MRUS,"Prompt")			From report interface Prompt
9	>	CONTAINS	TEXT	(121071,DCM,"Findings")			From report interface Findings
10	>	CONTAINS	CONTAINER	(T-45100, SNM3, Common carotid artery)			
11	>>	CONTAINS	CONTAINER	(FG3495-01, MRUS, Plaque Description)			
12	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
13	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
14	>>	CONTAINS	CONTAINER	(FG3495-02, MRUS, Plaque Area)			
15	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			

16	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
17	>	CONTAINS	CONTAINER	(T-45160,SRT,Carotid Bifurcation)			
18	>>	CONTAINS	CONTAINER	(FG3495-01, MRUS, Plaque Description)			
19	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
20	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
21	>>	CONTAINS	CONTAINER	(FG3495-02, MRUS, Plaque Area)			
22	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			

23 >>>

3	>	HAS CONCEPT MOD	CODE	EV (125101,		DCID (12117) Vessel Branch Modifiers	
4	>	CONTAINS	INCLUDE	DTID (300) Measurement		$Measurement = DCID (12119) Vascular Ultrasound Property $Derivation = DCID (3627) Measurement Type	
5	>>	HAS CONCEPT MOD	CODE	EV (R-4089A,		DCID (12233) Cardiac Phase	
6	>>	HAS CONCEPT MOD	CODE	EV (R-41FFC, period related to		DT (G-A491, SRT, "Post-prandial")	

C.7. CID (12104) Extracranial Arteries

CSD	CV	Code Meaning
SRT	T-45170	Carotid Bulb
SRT	T-45100	Common Carotid Artery
SRT	T-45200	External Carotid Artery
SRT	T-45300	Internal Carotid Artery
SRT	T-46100	Subclavian Artery
SRT	T-45700	Vertebral Artery

C.8. CID (12105) Intracranial Cerebral Vessels

CSD	CV	Code Meaning
SRT	T-45540	Anterior Cerebral Artery
SRT	T-45600	Middle Cerebral Artery
SRT	T-45900	Posterior Cerebral Artery
SRT	T-45320	Posterior Communicating Artery

C.9. CID (12106) Intracranial Cerebral Vessels (unilateral)

CSD	CV	Code Meaning
SRT	T-45800	Basilar Artery
SRT	T-45530	Anterior Communicating Artery
MRUS	V12106-01	Basilar Vein

C.10. CID (12107) Upper Extremity Arteries

CSD	CV	Code Meaning
SRT	T-47100	Axillary Artery
SRT	T-47160	Brachial Artery
SRT	T-47300	Radial Artery
SRT	T-46100	Subclavian Artery
SRT	T-47200	Ulnar Artery

C.11. CID (SELFCID-2) Upper Extremity Arteries(unilateral)

CSD	CV	Code Meaning
SRT	T-46010	Innominate Artery

C.12. CID (12108) Upper Extremity Veins

CSD	CV	Code Meaning
SRT	T-49110	Axillary vein
SRT	T-48052	Basilic vein
SRT	T-49350	Brachial vein
SRT	T-49240	Cephalic vein
SRT	T-49340	Radial vein
SRT	T-48330	Subclavian vein
SRT	T-49330	Ulnar vein

C.13. CID (12109) Lower Extremity Arteries

CSD	CV	Code Meaning
SRT	T-46710	Common Iliac Artery
SRT	T-47700	Anterior Tibial Artery
SRT	T-47400	Common Femoral Artery

CSD	CV	Code Meaning
SRT	T-47741	Dorsalis Pedis Artery
SRT	T-46910	External Iliac Artery
SRT	T-46740	Internal Iliac Artery
SRT	T-47630	Peroneal Artery
SRT	T-47500	Popliteal Artery
SRT	T-47600	Posterior Tibial Artery
SRT	T-47440	Profunda Femoris Artery
SRT	T-47403	Superficial Femoral Artery
MRUS	V12109-01	TP Trunk Artery

C.14. CID (12110) Lower Extremity Veins

CSD	CV	Code Meaning
SRT	T-49630	Anterior Tibial Vein
SRT	G-035B	Common Femoral Vein
SRT	T-48920	Common Iliac Vein
SRT	T-48930	External Iliac Vein
SRT	T-4942D	Gastrocnemius vein
SRT	T-49530	Great Saphenous Vein
SRT	T-49550	Lesser Saphenous Vein
SRT	T-49650	Peroneal Vein
SRT	T-49640	Popliteal Vein
SRT	T-49620	Posterior Tibial Vein
SRT	T-49660	Profunda Femoris Vein
SRT	G-036B	Soleal vein
SRT	G-035A	Superficial Femoral Vein
SRT	T-48940	Internal iliac vein
SRT	T-49410	Femoral vein
MRUS	V12110-01	TP Trunk Vein

C.15. CID (12112) Abdominal Arteries (unilateral)

CSD	CV	Code Meaning
SRT	T-42000	Aorta
SRT	T-46400	Celiac Axis

CSD	CV	Code Meaning
SRT	T-46421	Common Hepatic Artery
SRT	T-46422	Proper Hepatic Artery
SRT	T-46460	Splenic Artery
SRT	T-46510	Superior Mesenteric Artery
MRUS	C12120-1	Superior Mesenteric Artery/Aorta velocity ratio
MRUS	C12120-1	Celiac Artery/Aorta velocity ratio

C.16. CID (12114) Abdominal Veins (unilateral)

CSD	CV	Code Meaning
SRT	T-48720	Hepatic Vein
SRT	T-48727	Left Hepatic Vein
SRT	T-48725	Right Hepatic Vein
SRT	T-48726	Middle Hepatic Vein
SRT	T-48810	Portal Vein
SRT	T-48710	Inferior Vena Cava
SRT	T-48890	Splenic Vein
SRT	T-48840	Superior Mesenteric Vein
MRUS	V12114-01	Main Portal Vein

C.17. CID (12115) Renal Vessels

CSD	CV	Code Meaning
SRT	T-46600	Renal Artery
SRT	T-48740	Renal Vein
SRT	T-46659	Segmental Artery
SRT	T-4668A	Arcuate Artery of the Kidney
SRT	T-4667D	Interlobar Artery of Kidney
MRUS	V12115-01	Main Renal Artery
LN	33869-9	Renal Artery/Aorta velocity ratio

C.18. CID (12116) Vessel Segment Modifiers

CSD	CV	Code Meaning
SRT	G-A119	Distal
SRT	G-A188	Mid-longitudinal
SRT	G-036A	Origin of vessel

CSD	CV	Code Meaning
SRT	G-A118	Proximal

ICA	T-45300,SRT,Internal Carotid Artery
Subclav A	T-46100,SRT,Subclavian Artery
Vert A	T-45700,SRT,Vertebral Artery

C.19.3. Intracranial Cerebral Vessels

MODALITY Label	*DICOM Mapping*
ACA	T-45540,SRT,Anterior Cerebral Artery
MCA	T-45600,SRT,Middle Cerebral Artery
PCA	T-45900,SRT,Posterior Cerebral Artery
PComA	T-45320,SRT,Posterior Communicating Artery

C.19.4. Intracranial Cerebral Vessels (unilateral)

MODALITY Label	*DICOM Mapping*
BA	T-45800,SRT,Basilar Artery
AComA	T-45530,SRT,Anterior Communicating Artery
Ba V	V12106-01,MRUS,Basilar Vein

C.19.5. Upper Extremity Arteries

MODALITY Label	*DICOM Mapping*
Axill A	T-47100,SRT,Axillary Artery
Brachial	T-47160, SRT, Brachial Artery
Radial A	T-47300,SRT,Radial Artery
Subclav	T-46100, SRT, Subclavian Artery
Ulnar A	T-47200,SRT ,Ulnar Artery

C.19.6. Upper Extremity Arteries(unilateral)

MODALITY Label	*DICOM Mapping*
Innom A	T-46010, SRT, Innominate Artery

C.19.7. Upper Extremity Veins

MODALITY Label	*DICOM Mapping*
Axill V	T-49110,SRT ,Axillary vein

Cephalic V