DICOM CONFORMANCE STATEMENT

FOR

DP-50/DP-50T/DP-50Expert/DP-50 Pro/DP-50 PT/DP-50S/DP-50 Vet

DIGITAL ULTRASONIC DIAGNOSTIC IMAGING SYSTEM

1 Conformance Statement Overview

This document describes the conformance to the DICOM 3.0(NEMA PS 3.1-3.18(2009), Digital Imaging and Communication in Medicine (DICOM) Set by all the ultrasound systems such as DP-50/DP-50T/DP-50Expert/DP-50Pro/DP-50 PT/DP-50S/DP-50 Vet. We specify ultrasound system generally refer to the products above in this document. The ultrasound system implements the necessary DICOM services to download worklists from an information system, save acquired Ultrasound (US) images and associated Structured Reports to a network storage device and/or removable media, print to a networked hardcopy device, query and retrieve the US images from a networked storage system, and inform the information system about the works actually done. Table 1 provides an overview of the supported network services, Table 2 lists the supported Media Storage Application Profiles, and Table 3 lists the supported Structured Report Templates.

Table 1
NETWORK SERVICES

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Transfer Storage		
Verification	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
Secondary Capture Image Storage	Yes	Yes
Query/Retrieve		
Study Root Query/Retrieve Information Model FIND[1]	Yes	No
Study Root Query/Retrieve Information Model MOVE[1]	Yes	No
Workflow Management		
Modality Worklist Information Model Find[1]	Yes	No
Modality Performed Procedure Step[1]	Yes	No
Storage Commitment Push Model	Yes	No
Print Management		
Basic Color Print Management	Yes	No

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Basic Grayscale Print Management	Yes	No
Notes, Reports, Measurements, Transfer[1]		
Comprehensive SR Storage[1]	Yes	Yes

Table 2
MEDIA SERVICES

Media Storage Application Profile	Write Files (FSC / FSU)	Read Files (FSR)
Compact Disk - Recordable		
STD-US-SC-SF&MF-CDR	Yes / Yes[2]	Yes
DVD		
STD-US-SC-SF&MF-DVD STD-US-SC-SF&MF-DVD-RAM	Yes / Yes[2]	Yes
USB Devices		
STD-GEN-USB-JPEG for Ultrasound images, compressed and uncompressed and Structured Reports	Yes / Yes[2]	Yes

Table 3
STRUCTURED REPORTS

Concept Name	Supported
OB-GYN Ultrasound Procedure Report[1]	Yes
Echocardiography Procedure Report[1]	Yes
Vascular Ultrasound Report[1]	Yes

Note:
1 The function is not available in DP-50 Vet.
2 Only acts as a FSU for media that may be written to multiple times.

2 Table of Contents

1 Conformance Statement Overview I
2 Table of Contents III
3 Introduction 1
3.1 Review History 1
3.2 Audience 1
3.3 Remarks 1
3.4 Terms and Definitions 2
3.5 Acronyms, Abbreviations, and Symbols 4
3.6 References 5
4 Networking 6
4.1 Implementation Model 6
4.1.1 Application Data Flow 6
4.1.2 7
4.1.3 Sequence of Real World Activities 11
4.2 AE Specifications 12
4.2.1 Modality AE 12
4.3 Network Interface 59
4.3.1 Supported Communications Stacks 59
4.3.2 TCP/IP Stack 59
4.3.3 Physical Network Interface 59
4.3.4 Additional Protocols 60
4.4 Configuration 60
4.4.1 AE Title/Presentation Address Mapping 60
4.4.2 Configurable Parameters 60
5 Media Storage 65
5.1 Implementation Model 65

8.1.1 Created SOP Instances 73
8.1.2 73
8.1.3 Attribute Mapping 73
8.1.4 Coerced/Modified fields 73
8.2 Data Dictionary of private attributes 73
8.3 Coded terminology and templates 73
8.4 Grayscale Image Consistency 73
8.5 Standard extended/specialized/private sop Classes 74
8.6 Private Transfer Syntaxes 74
A. Appendix : OB GYN structured reporting template 75
A.1. TID (300) Measurement 75
A.2. TID 1008 Subject Context, Fetus 76
A.3. TID (5000) OB-GYN Ultrasound Procedure Report 76
A.4. TID (SELFTMP-1) Fetal Cardiac Measurement Group 78
A.5. TID (SELFTMP-2) Fetal ZScore 78
A.6. TID (1001) OBSERVATION CONTEXT 79
A.7. TID (5001) OB-GYN Patient Characteristics 80
A.8. TID (5002) OB-GYN Procedure Summary 80
A.9. TID (5003) OB-GYN Fetus Summary 82
A.10. TID (FINDING_1) Fetal Description 83
A.11. TID (FINDING_2) Fetus Limbs 85
A.12. TID (FINDING_3) Fetal Cardiology 85
A.13. TID (FINDING_4) Fetal Brain 85
A.14. TID (FINDING_5) Spine 86
A.15. TID (FINDING_6) Fetal Environment 86
A.16. TID (FINDING_7) Maternal Description 87
A.17. TID (5004)Fetal Biometry Ratio Section 87
A.18. TID (5005) Fetal Biometry Section 88

A.37. CID (12009) Early Gestation Biometry Measurements 101
A.38. CID (12013) Gestational Age Equations and Tables 101
A.39. CID (12014) Fetal Body Weight 103
A.40. CID (12015) Fetal Growth Equations and Tables 104
A.41. CID (12119) Vascular Ultrasound Property 106
A.42. CID (12120) Blood Velocity Measurements 107
A.43. CID (12121) Vascular Indices and Ratios 107
A.44. CID (12122) Other Vascular Properties 107
A.45. CID (12140) Pelvic Vasculature Anatomical Location 108
A.46. CID (12141) Fetal Vasculature Anatomical Location 108
A.47. CID (SELFCID-1) Fetal Z-Score 108
A.48. Mapping between Modality measurements and DICOM Concepts. 109
A.48.1. OB-GYN Measurements 109
A.48.2. Vasculature Anatomic Location 114
A.48.3. OB-GYN Vascular Measurements 114
A.48.4. OB-GYN Cardic Measurements 115
A.48.5. Biophysical Profile Measurements 116
B. Appendix : Cardiac structured reporting template 118
B.1. TID (5200) Echocardiography Procedure Report 118
B.2. TID(1001) Observation Context 121
B.3. TID (5201) Echocardiography Patient Characteristics 122
B.4. TID (SELFTMP-2) Echo Procedure Summary Section 123
B.5. TID (5202) ECHO SECTION 124
B.6. TID (5203) Echo Measurement 124
B.7. CID (12200) Echocardiography Left Ventricle 126
B.8. CID (12201) Left Ventricle Linear 126
B.9. CID (12202) Left Ventricle Volume 126
B.10. CID (12203) Left Ventricle Other 127
B.11. CID (12204) Echocardiography Right Ventricle 127
B.12. CID (12205) Echocardiography Left Atrium 128
B.13. CID (12206) Echocardiography Right Atrium 128
B.14. CID (12207) Echocardiography Mitral Valve 128
B.15. CID (12208) Echocardiography Tricuspid Valve 130
B.16. CID (12209) Echocardiography Pulmonic Valve 130
B.17. CID (12210) Echocardiography Pulmonary Artery 130
B.18. CID (12211) Echocardiography Aortic Valve 130
B.19. CID (12212) Echocardiography Aorta 131
B.20. CID (12214) Echocardiography Pulmonary Veins 131
B.21. CID (12215) Echocardiography Vena Cavae 131
B.22. CID (12217) Echocardiography Cardiac Shunt 132
B.23. CID (12218) Echocardiography Congenital 132
B.24. CID (12220) Echocardiography Common Measurements 132
B.25. CID (12221) Flow Direction 133
B.26. CID (12222) Orifice Flow Properties 133
B.27. CID (12224) Ultrasound Image Modes 134
B.28. CID (12226) Echocardiography Image View 134

B.29. CID (12227) Echocardiography Measurement Method 134
B.30. CID (12228) Volume Methods 135
B.31. CID (12229) Area Methods 135
B.32. CID (12230) Gradient Methods 135
B.33. CID (12231) Volume Flow Methods 136
B.34. CID (12232) Myocardium Mass Methods 136
B.35. CID (12233) Cardiac Phase 136
B.36. CID (12234) Respiration Phase 136
B.37. CID (12239) Cardiac Output Properties 136
B.38. CID (12240) Left Ventricle Area 136
B.39. CID (90000) Pericardial disease 137
B.40. Mapping between Modality measurements and DICOM Concepts. 137
B.40.1. Left Ventricle Measurements 137
B.40.2. Right Ventricle Measurements 154
B.40.3. Left Atrium Measurements 155
B.40.4. Right Atrium Measurements 156
B.40.5. Aortic Valve Measurements 157
B.40.6. Mitral Valve Measurements 159
B.40.7. Pulmonic Valve Measurements 164
B.40.8. Tricuspid Valve Measurements 166
B.40.9. Aorta Measurements 168
B.40.10. Pulmonary Artery Measurements 169
B.40.11. Vena Cava Measurements 169
B.40.12. Pulmonary Venous Structure Measurements 170
B.40.13. Cardiac Shunt Study Measurements 171
B.40.14. Congenital Anomaly of Cardiovascular System Measurements 171
B.40.15. Pericardial Disease Measurements 172
B.40.16. Heart Rate Measurements 172
C. Appendix : Vascular structured reporting template 173
C.1. TID (5100) Vascular Ultrasoud Report 173
C.2. TID (1001) Observation Context 179
C.3. TID (5101) Vascular Patient Characteristics 180
C.4. TID (5102) Vascular Procedure Summary Section 181
C.5. TID (5103) Vascular Ultrasound Section 183
C.6. TID (5104) Vascular Ultrasound Measurement Group 183
C.7. CID (12104) Extracranial Arteries 184
C.8. CID (12105) Intracranial Cerebral Vessels 184
C.9. CID (12106) Intracranial Cerebral Vessels (unilateral) 184
C.10. CID (12107) Upper Extremity Arteries 185
C.11. CID (SELFCID-2) Upper Extremity Arteries(unilateral) 185
C.12. CID (12108) Upper Extremity Veins 185
C.13. CID (12109) Lower Extremity Arteries 185
C.14. CID (12110) Lower Extremity Veins 186
C.15. CID (12112) Abdominal Arteries (unilateral) 186
C.16. CID (12114) Abdominal Veins (unilateral) 187
C.17. CID (12115) Renal Vessels 187

C.18. CID (12116) Vessel Segment Modifiers 187
C.19. Mapping between Modality measurements and DICOM Concepts. 188
C.19.1. Vascular Measurements 188
C.19.2. Extracranial Arteries 188
C.19.3. Upper Extremity Arteries 189
C.19.4. Upper Extremity Arteries(unilateral) 189
C.19.5. Upper Extremity Veins 189
C.19.6. Lower Extremity Arteries 189
C.19.7. Lower Extremity Veins 190
C.19.8. Abdominal Arteries (unilateral) 190
C.19.9. Abdominal Veins (unilateral) 190
C.19.10. Renal Vessels 191

3 Introduction

3.1 Review History

DOCUMENT VERSION	DATE OF ISSUE	DESCRIPTION
1.0	Oct. 26, 2011	Creation of the document

3.2 Audience

This document is intended for potential customers, system integrators of medical equipment, marketing staff interested in system functionality and software designers implementing DICOM interfaces. It is assumed that the readers of this document are familiar with the DICOM Standard and with the terminology and concept which are used in the Standard. If readers are unfamiliar with DICOM terminology they should read the DICOM Standard, prior to reading this DICOM Conformance Statement document.

3.3 Remarks

The scope of this DICOM Conformance Statement is to facilitate integration between Mindray Products and other DICOM products. The Conformance Statement should be read and understood in conjunction with the DICOM Standard. DICOM by itself does not guarantee interoperability. The Conformance Statement does, however, facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.

This Conformance Statement is not supposed to replace validation with other DICOM equipment to ensure proper exchange of intended information. In fact, the user should be aware of the following important issues:

The comparison of different Conformance Statements is the first step towards assessing interconnectivity and interoperability between Mindray medical equipment and other DICOM conformant equipments.

Test procedures should be defined and executed to validate the required level of interoperability with specific compatible DICOM equipment, as established by the healthcare facility.

actively involved in the development of the DICOM standard. Therefore, Mindray reserves the right to make changes to its products or to discontinue its delivery.

The Ultrasound System follows the IHE SWF, PDI, ED Profiles.

3.4 Terms and Definitions

- **Abstract Syntax** the information agreed to be exchanged between applications, generally equivalent to a Service/Object Pair (SOP) Class. Examples: Verification SOP Class, Modality Worklist Information Model Find SOP Class, Computed Radiography Image Storage SOP Class.
- **Application Context** the specification of the type of communication used between *Application Entities*. Example: DICOM network protocol.
- **Application Entity (AE)** an end point of a DICOM information exchange, including the DICOM network or media interface software; i.e., the software that sends or receives DICOM information objects or messages. A single device may have multiple Application Entities.
- **Application Entity Title** the externally known name of an *Application Entity*, used to identify a DICOM application to other DICOM applications on the network. The Called AE Title defines the intended receiver of an Association. Nevertheless, the Calling AE Title defines the requestor of an Association.
- **Association** a network communication channel set up between *Application Entities*.
- **Association Establishment** - an Association Establishment is the first phase of communication between two DICOM Application Entities. The AEs use the Association Establishment to negotiate how data will be encoded and the type of data to be exchanged.
- **Attribute** a unit of information in an object definition; a data element identified by a *tag*. The information may be a complex data structure (Sequence), itself composed of lower level data elements. Examples: Patient ID (0010,0020), Accession Number (0008,0050), Photometric Interpretation (0028,0004), Procedure Code Sequence (0008,1032).
- **DICOM File Format** - the DICOM File Format provides a means to encapsulate in a File the Data Set representing a SOP Instance related to a DICOM Information Object.
- **DICOM Message Service Element (DIMSE)** a DIMSE defines the services and protocols utilized by an Application Entity to exchange messages.
- **File** - a File is an ordered string of zero or more bytes, where the first byte is at the beginning of the file and the last byte is at the end of the File. Files are identified by an unique File ID and may by written, read, or deleted.
- **File Meta Information** - the File Meta Information includes identifying information on the encapsulated Data Set. It is a mandatory header at the beginning of every DICOM File.
- **Information Object Definition (IOD)** - the specified set of *Attributes* that comprise a type of data object; does not represent a specific instance of the data object, but rather a class of similar data objects that have the same properties. The *Attributes*

may be specified as Mandatory (Type 1), Required but possibly unknown (Type 2), or Optional (Type 3), and there may be conditions associated with the use of an Attribute (Types 1C and 2C). Examples: Print Job IOD.

- **Joint Photographic Experts Group (JPEG)** a set of standardized image compression techniques, available for use by DICOM applications.
- **Module** a set of *Attributes* within an *Information Object Definition* that are logically related to each other. Example: Patient Module includes Patient Name, Patient ID, Patient Birth Date, and Patient Sex.
- **Negotiation** first phase of *Association* establishment that allows *Application Entities* to agree on the types of data to be exchanged and how that data will be encoded.
- **Physical Media** - a piece of material with recording capabilities for streams of bits. Characteristics of a Physical Media include form factor, mechanical characteristics, recording properties and rules for recording and organizing bit streams in accessible structures.
- **Presentation Context** the set of DICOM network services used over an *Association*, as negotiated between *Application Entities*; includes *Abstract Syntaxes* and *Transfer Syntaxes*.
- **Protocol Data Unit (PDU)** a packet (piece) of a DICOM message sent across the network. Devices must specify the maximum size packet they can receive for DICOM messages.
- **Security Profile** a set of mechanisms, such as encryption, user authentication, or digital signatures, used by an *Application Entity* to ensure confidentiality, integrity, and/or availability of exchanged DICOM data.
- **Service Class Provider (SCP)** role of an *Application Entity* that provides a DICOM network service; typically, a server that performs operations requested by another *Application Entity* (*Service Class User*). Examples: Picture Archiving and Communication System (image storage SCP, and image query/retrieve SCP), Radiology Information System (modality worklist SCP).
- **Service Class User (SCU)** role of an *Application Entity* that uses a DICOM network service; typically, a client. Examples: imaging modality (image storage SCU, and modality worklist SCU), imaging workstation (image query/retrieve SCU).
- **Service/Object Pair (SOP) Class** the specification of the network or media transfer (service) of a particular type of data (object); the fundamental unit of DICOM interoperability specification. Examples: Ultrasound Image Storage Service, Basic Grayscale Print Management.
- **Service/Object Pair (SOP) Instance** an information object; a specific occurrence of information exchanged in a *SOP Class*. Examples: a specific x-ray image.
- **Tag** a 32-bit identifier for a data element, represented as a pair of four digit

the tag is for a private (manufacturer-specific) data element. Examples: (0010,0020) [Patient ID], (07FE,0010) [Pixel Data], (0019,0210) [private data element].

4 Networking

4.1 Implementation Model

4.1.1 Application Data Flow

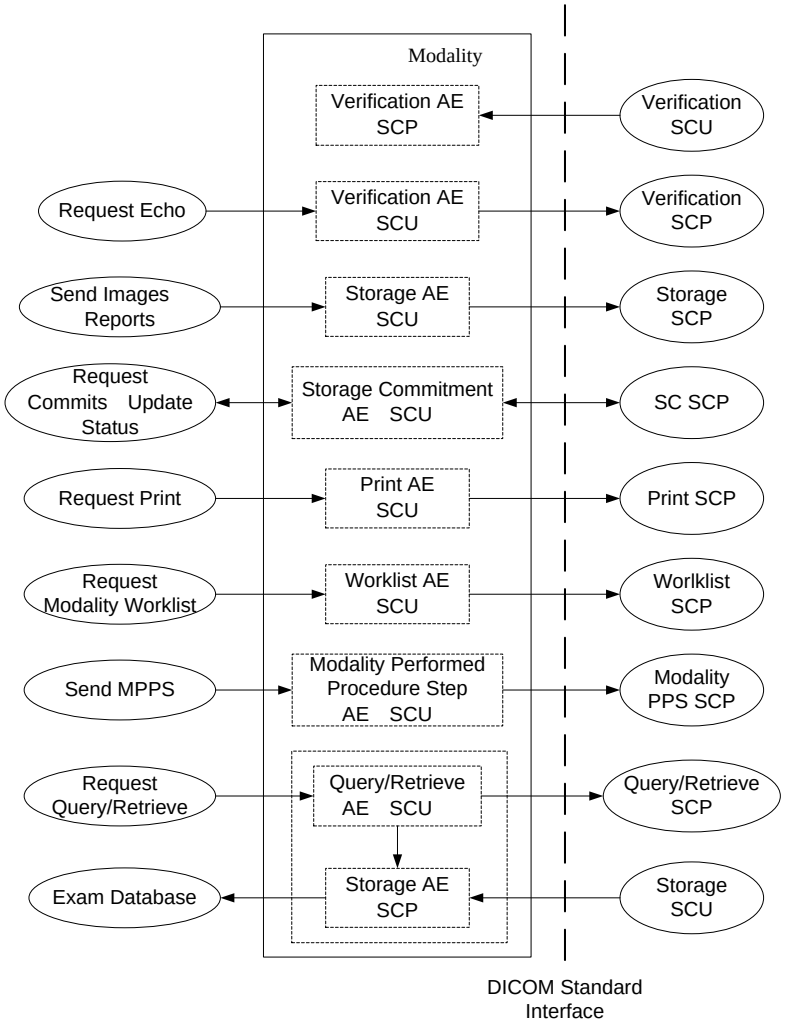

Figure 1

Implementation Model

Note Storage AE SCP only be used in Query/Retrieve.

This application entity provides a user interface, internal database and network listener that spawns additional threads as necessary to handle incoming connections.

Conceptually the network services may be modeled as the following AEs, however, in fact all the AEs share a single (configurable) AE Title:

- Verification AE (as SCU and SCP)

- Operation 1

Step 1: Select the images from thumbnail menu in main UI.

SCPs.

Step 3: Send the image to the DICOM Storage service SCPs.

- Operation 2

Step 1: Select exams in the iStation Dialog.

Step 2: Pr Exam and select DICOM Storage service.

Step 3: Send the selected exams (maybe include images, SRs) to the DICOM Storage service SCPs.

- Operation 3

Step 1: Select thumbnail in the iStation Dialog.

Step 2: SCPs.

Step 3: Send the image to the DICOM Storage service SCPs.

- Operation 4

Step 1: Open the review dialog and select the images.

Step 2: P the storage SCPs.

Step 3: Send the image to the DICOM Storage service SCPs.

The SR only could be sent in the circumstance as below:

- The exam type is obstetric, gynecology, cardiac, vascular,
- The SR Key for the exam type must be installed in option preset UI.
- Exam is the unit to send.
- The status of the exam is "End", "Paused" or "Cancelled". SR would not be sent when an active exam is selected.
- The DICOM storage service SCPs should be set as "Attach SR when Store Images" or "Only Store SR".

In the event that the ultrasound system is taken off the network as a portable system or when a network failure occurs during a background store, the Storage SCU maintains a queue of failed C-STORE requests. If pre-configured on Preset UI, the failed C-Store requests will be automatically retried specified times. If no pre-configuration, the user can also retry the failed requests manually.

As a SCP, the Storage AE could only be used in Query/Retrieve, otherwise couldn't.

4.1.2.3 Storage Commitment AE

The Storage Commitment AE originates associations to ensure the reliable storage of

print service SCPs.

Step 3: Send the image to the DICOM print service SCPs.

- Operation 2

Step 1: Select exams in the iStation Dialog.

Step 2: Pr Exam and select DICOM print service SCPs.

Step 3: Send the single frame images and secondary capture images of the selected exams to the DICOM print service SCPs.

- Operation 3

Step 1: Select thumbnail in the iStation Dialog.

Step 2: t DICOM print service SCPs.

Step 3: Send the image to the DICOM print service SCPs.

- Operation 4

Step 1: Open the review dialog and select the images.

Step 2: P print SCPs.

Step 3: Send the image to the DICOM print service SCPs.

4.1.2.5 Worklist AE

The Worklist AE is activated through the Worklist UI when the user selects a remote AE to query (from a pre-configured list).The system supports automatic and manual query depending on its configuration on Preset UI. The system supports fuzzy query using ? and * .

- If set one and only one remote AE to be default status. The system can initiate a query with default rules when show the Worklist UI. The Worklist Server is the default server. The Modality Type is US, the Exam Date is today, and the Scheduled Station AE Title is blank.
- Alternatively if the default status is no, the user can specify query rules on Worklist UI. Such as Patient ID, Patient Name, Accession Number, Requested Procedure ID, Worklist Server, Exam Date, Modality Type and Scheduled Station AE Title.

If no matches are found, a dialogue will be presented to the user to indicate so. The possible reasons for this failure are listed to help trouble shorouble al ae lTBe BT1 (y)23(m[(D)-4(l)5(ch)-11(e

4.1.2.6 MPPS AE

MPPS AE sends event transactions that facilitate the transfer of exam procedure status from the ultrasound system to the information system.

MPPS messages are sent from the system under the following circumstances:

- MPPS N-Create, Status = IN PROGRESS. Starting a new exam or reactive an exam result in automated creation of an MPPS Instance managed by a remote AE.
- MPPS N-Set, Status = COMPLETE. Completion of the MPPS is performed as the result of an operator action of ending the exam.
- MPPS N-Set, Status = DISCONTINUED. Exam status to be sent. User can select various reasons from the Reason of cancel Exam UI when need to cancel an exam.

4.1.2.7 Query/Retrieve AE

The Query/Retrieve AE supports the Query/Retrieve services as an SCU.

As a Query SCU, the system initiates a C-Find request to the remote SCP if pre-configured on the Preset UI, and then query is invoked directly by the user. The system supports fuzzy query using ? and * .

For remote AE, no matter what the default status is, the user can specify query rules on Query/Retrieve UI. Such as Patient ID, Patient Name, Accession Number, Exam Date and select Search Key. If no matches are found, a dialogue will be presented to the user to indicate so. The user can also change query rules for another query, or for further filter in local database to locate the patients quickly.

As a Move SCU, the system supports the Study Root Query Model. The stystem can only retrieve ultrasound images or structed reports, whose modality atrributes are "US" or "SR", but will leap all the other ones. Furthermore, the retrieval destination is only local host.

The system initiates a C-MOVE request to the remote Retrieve SCP when user selects items to retrieve. The remote Retrieve SCP in turn starts C-STORE sub operations to the ultrasound system.

User can discover lists number for queried items, as well as retrieval items. And the lists can be sorted in ascending or descending order.

4.2 AE Specifications

4.2.1 Modality AE

4.2.1.1 SOP Classes

The ultrasound system provides Standard Conformance to the following SOP Class:

Table 4
SOP Class for Modality AE

SOP Class Name	SOP Class UID	SCU	SCP
Verification SOP Class	1.2.840.10008.1.1	Yes	Yes
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes[1]
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes[1]
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes[1]
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	Yes[1]
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	Yes	No
Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Yes	No
Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No
Print Job SOP Class	1.2.840.10008.5.1.1.14	Yes	No
Modality Worklist Information Model Find	1.2.840.10008.5.1.4.31	Yes	No
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Yes	No
Study Root Query/Retrieve Information Model - Find	1.2.840.10008.5.1.4.1.2.2.1	Yes	No
Study Root Query/Retrieve Information Model - Move	1.2.840.10008.5.1.4.1.2.2.2	Yes	No

Note 1 Yes only used in Query/Retrieve, otherwise No.

4.2.1.2 Association Establishment Policies

4.2.1.2.1General

The DICOM standard application context name for DICOM 3.0 is always proposed:

Table 5
DICOM Application Context for Modality AE

Figure 2
Sequencing of Activity Send Echo Request

4.2.1.3.1.2 Proposed Presentation Contexts

The Verification AE (as SCU) supports the following Presentation Contexts for Verification.

Table 9
Presentation Contexts for Verification

PROPOSED PRESENTATION CONTEXTS					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name**	**UID**		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

4.2.1.3.1.33 SOP Specific Conformance

It summarizes the behavior of Ultrasound System when receiving status codes in a C-ECHO response.

Table 10
Verification C-Echo Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior (as SCU)
Success	Success	0000	Device Status is set to: Verify Successful
Refused	Out of Resources	A7XX	Device Status is set to: Verify Failed
Failed	Unable to process	CXXX	Device Status is set to: Verify Failed
*	*	Any other status code	Device Status is set to: Verify Failed

4.2.1.3.2 Activity Store images, SRs

4.2.1.3.2.1 Description and Sequencing of Activities

For each exam, images selected from the user interface will be transfered to the selected remote AE. When the storage fails, not only the failed task will automatically retry specific times if configured on Preset UI, but also user can restart the failed task by clicking the Retry Button on the ultrasound task management dialog. Besides that, in the event that the ultrasound system is taken off the netw1(n)11(t)5( )-3 648(m)-30( )] c7o6974.03 Tm[(111(a)11(g)-11(e)3 CTkuoG[(E)8(n)11(si)53(3T12.81)-3

Table 11

Proposed Presentation Contexts for Storage

PROPOSED PRESENTATION CONTEXTS					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name**	**UID**		
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCU	None
		RLE Lossless	1.2.840.10008.1.2.5	SCU	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCU	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCU	None
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCU	None
		RLE Lossless	1.2.840.10008.1.2.5	SCU	None
		JPEG 2000 Image Compression (Lossless	1.2.840.10008.1.2.4.90	SCU	None

		Only)			
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCU	None
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCU	None
		RLE Lossless	1.2.840.10008.1.2.5	SCU	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCU	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCU	None
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

Storage Communication Failure Behavior

Exception	Behavior
Timeout	The Association is aborted using A-ABORT and the send job is marked as failed. The reason is logged and the job failure is reported to the user via task management.
Association aborted by the SCP or network layers	The send job is marked as failed. The reason is logged and the job failure is reported to the user via task management.

The following table provides the list of attributes requested in the Storage.

Table 14

Storage IOD Attribute

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
Module: Patient Module (M)				
(0010,0010)	PN	2	Patient's Name	MWL/USER
(0010,0020)	LO	2	Patient ID	MWL/USER

				calculated automatically.
(0010,1020)	DS	3	Patient's Size	MWL/USER, default is set to zero length
(0010,1030)	DS	3	Patient's Weight	MWL/USER, default is set to zero length
(0010,21B0)	LT	3	Additional Patient History	MWL
Module: General Series Module (M)				
(0008,0021)	DA	3	Series Date	AUTO
(0008,0031)	TM	3	Series Time	AUTO
(0008,0060)	CS	1	Modality	
(0008,103E)	LO	3	Series Description	MWL
(0008,1050)	PN	3	Performing Physician's Name	MWL/USER, default is set to zero length
(0008,1070)	PN	3	Operators' Name	MWL/USER, default is set to zero length
(0018,1030)	LO	3	Protocol Name	AUTO set to ExamType
(0018,5100)	CS	2C	Patient Position	Set to zero length
(0020,000E)	UI	1	Series Instance UID	AUTO
(0020,0011)	IS	2	Series Number	AUTO
(0020,0060)	CS	2C	Laterality	Set to zero length
(0040,0244)	DA	3	Performed Procedure Step Start Date	MPPS
(0040,0245)	TM	3	Performed Procedure Step Start Time	MPPS
(0040,0254)	LO	3	Performed Procedure Step Description	MPPS
(0040,0260)	SQ	3	Performed Protocol Code Sequence	MPPS
Module: General Equipment Module (O)				
(0008,0070)	LO	2	Manufacturer	MINDRAY
(0008,0080)	LO	3	Institution Name	CONFIG
(0008,1010)	SH	3	Station Name	AUTO
(0008,1040)	LO	3	Institutional Department Name	CONFIG
(0008,1090)	LO	3	Manufacturer's Model Name	DP-50

(0018,1000)	LO	3	Device Serial Number	The Ethernet card Mac Address
(0018,1020)	LO	3	Software Version(s)	AUTO
Module: General Image Module (M)				
(0008,0023)	DA	2C	Content Date	AUTO
(0008,0033)	TM	2C	Content Time	AUTO
(0008,2111)	ST	3	Derivation Description	CONFIG, default is set to zero length
(0020,0013)	IS	2	Instance Number	AUTO
(0020,0020)	CS	2C	Patient Orientation	Set to zero length
(0020,4000)	LT	3	Image Comments	Set to zero length
(0028,0301)	CS	3	Burned In Annotation	YES
Module: US Image Module (M)				
(0008,0008)	CS	2	Image Type	ORIGINAL/PRIMARY
(0018,5010)	LO	3	Transducer Data	USER
(0018,5020)	LO	3	Processing Function	USER
(0028,0002)	US	1	Samples per Pixel	1 or 3
(0028,0004)	CS	1	Photometric Interpretation	RGB, for color images; MONOCHROME2, if the image is grayscale; YBR_FULL_422, if the image is sent using JPEG. RGB, if the image is sent using JPEG Lossless. YBR_FULL,if the image is sent using RLE Lossless. YBR_ICT,if the image is sent using JPEG 2000 Image Compression. YBR_RCT,if the image is sent using JPEG 2000 Image Compression (Lossless Only)
(0028,0006)	US	1C	Planar Configuration	1, if the image is sent using RLE Lossless 0 otherwise.
(0028,0009)	AT	1C	Frame Increment Pointer	Frame Time

(0028,0014)	US	3	Ultrasound Color Data Present	0 or 1
(0028,0100)	US	1	Bits Allocated	0x0008
(0028,0101)	US	1	Bits Stored	0x0008
(0028,0102)	US	1	High Bit	0x0007
(0028,0103)	US	1	Pixel Representation	0x0000
(0028,2110)	CS	1C	Lossy Image Compression	Not used if image is uncompressed; support JPEG baseline, JPEG Lossless,RLE Lossless,JPEG 2000 Image Compression,JPEG 2000 Image Compression (Lossless Only)
Module: Image Pixel Module (M)				
(0028,0010)	US	1	Rows	AUTO
(0028,0011)	US	1	Columns	AUTO
(0028,0034)	IS	1c	Pixel Aspect Ratio	Set to zero length
(7FE0,0010)	OW	1	Pixel Data	
Module: SOP Common Module (M)				
(0008,0005)	CS	1C	Specific Character Set	AUTO
(0008,0012)	DA	3	Instance Creation Date	AUTO
(0008,0013)	TM	3	Instance Creation Time	AUTO
(0008,0016)	UI	1C	SOP Class UID	AUTO
(0008,0018)	UI	1C	SOP Instance UID	AUTO
Module: US Region Calibration Module (U)				
(0018,6011)	SQ	1	Sequence of Ultrasound Regions	
>(0018,6012)	US	1	Region Spatial Format	Set by the system
>(0018,6014)	US	1	Region Data Type	Set by the system
>(0018,6016)	UL	1	Region Flags	Set by the system
>(0018,6018)	UL	1	Region Location Min X0	Set by the system
>(0018,601A)	UL	1	Region Location	Set by the system

			Min Y0	
>(0018,601C)	UL	1	Region Location Max X1	Set by the system
>(0018,601E)	UL	1	Region Location Max Y1	Set by the system

(0018,1016)	LO	3	Secondary Capture Device Manufacturer	MINDRAY
(0018,1018)	LO	3	Secondary Capture Device Manufacturer's Model Name	DP-50
(0018,1019)	LO	3	Secondary Capture Device Software Version(s)	AUTO
Module: SC Image Module (M) **Used for Second Capture Images Only**				
(0018,1012)	DA	3	Date of Secondary Capture	AUTO
(0018,1014)	TM	3	Time of Secondary Capture	AUTO

Conventions used for the Value(s) and Comments section are:

MWL the attribute value source is from Modality WORKLIST

USER

AUTO automatically generated by the MODALITY system

CONFIG - the attribute value source is a configurable parameter

4.2.1.3.3 Activity Film Images

4.2.1.3.3.1 Description and Sequencing of Activities

A user composes images onto film sheets and requests them to be sent to a specific hardcopy device. The user can select the desired film format and number of copies. Each print-job is forwarded to the job queue and processed individually.

The system is invoked by the user on Send to UI if the print remote AE is pre-configured. Status of the print-job is reported through task management UI. If pre-configured on Preset UI, the failed print task will be automatically retried specified times. If no pre-configuration, the user can also retry manually. Only one task will be active at a time for each separate hardcopy device. The same as Storage, the system could retry automaticlly the failed task caused by network failure when the network is restored.

A typical sequence of DIMSE messages sent over an association between Print AE and a Printer is illustrated in Figure 4:

1. Print AE opens an association with the Printer.
2. N-GET on the Printer SOP Class is used to obtain current printer status information.
3. N-CREATE on the Film Session SOP Class creates a Film Session.
4. N-CREATE on the Film Box SOP Class creates a Film Box linked to the Film Session. A single Image Box will be created as the result of this operation (Print AE default

uses the format STANDARD\1.1, but user can change it on Preset UI).

5. N-SET on the Image Box SOP Class transfers the contents of the film sheet to the printer.
6. N-ACTION on the Film Box SOP Class instructs the printer to print the Film Box.
7. The Printer prints the requested number of film sheets.
8. The Printer asynchronously reports its status via N-EVENT-REPORT notification (Printer SOP Class). The Printer can send this message at any time. Print AE does not require the N-EVENT-REPORT to be sent. Print AE is capable of receiving an N-EVENT-REPORT notification at any time during an association.
9. N-DELETE on the Film Box SOP Class deletes the complete Film box SOP Instance hierarchically.
10. N-DELETE on the Film Session SOP Class deletes the complete Film Session SOP Instance hierarchically.
11. Print AE closes the association with the Printer.

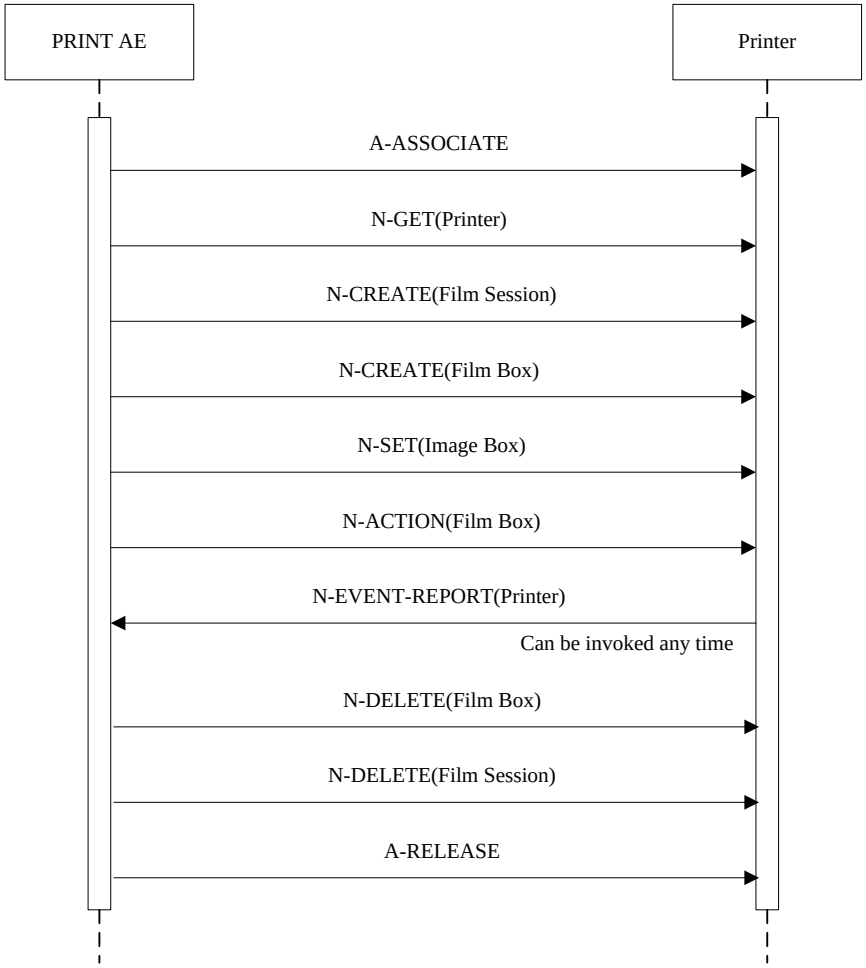

Figure 4

Sequencing of Activity Film Images

4.2.1.3.3.2 Proposed Presentation Contexts

Print AE is capable of proposing the Presentation Contexts shown in the Table below:

Table 15
Proposed Presentation Contexts for Activity Film Images

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

4.2.1.3.3.3 Common SOP Specific Conformance for all Print SOP Classes

The general behavior of Print AE during communication failure is summarized in the Table below. This behavior is common for all SOP Classes supported by Print AE.

Table 16
Print AE Communication Failure Behavior

Exception	Behavior
Timeout	The association is aborted using A-ABORT and the print-job is marked as failed.
Association aborted by the SCP or network layers	The print-job is marked as failed. The reason is logged and the job failure is reported to the user.

Recommended abbreviations to be used for the tables are:

VNAP Value Not Always Present (attribute sent zero length if no value is present)

ANAP Attribute Not Always Present

ALWAYS Always Present with a value

EMPTY Attribute is sent without a value

Recommended abbreviations to be used for the source of the data values in the tables are:

			print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.4.2 Printer SOP Class Notifications (N-EVENT-REPORT)

Table 19

Printer SOP Class N-Event-Report Behavior

Event Type Name	Event Type ID	Behavior
Normal	1	The print-job continues to be printed.
Warning	2	The print-job continues to be printed. The contents of Printer Status Info (2110, 0020) is logged and reported to the user via the job-control application.
Failure	3	The print-job is marked as failed. The contents of Printer Status Info (2110, 0020) is logged and reported to the user via the job-control application.
*	*	An invalid Event Type ID will cause a status code of 0113H to be returned in a N-EVENT-REPORT response.

Print AE is capable of receiving an N-EVENT-REPORT request at any time during an association. The behavior of Print AE when receiving Event Types within the N-EVENT-REPORT is summarized in the Table 19.

The reasons for returning specific status codes in a N-EVENT-REPORT response are summarized in the Table below:

Table 20

Printer SOP Class N-EVENT-REPORT Response Status Reasons

Service Status	Further Meaning	Error Code	Reasons
Success	Success	0000	The notification event has been successfully received.
Failure	No Such Event Type	0113H	An invalid Event Type ID was supplied in the N-EVENT-REPORT request.
Failure	Processing Failure	0110H	An internal error occurred during processing of the N-EVENT-REPORT. A short description of the error will be returned in Error Comment (0000, 0902).

4.2.1.3.3.5 SOP Specific Conformance for the Film Session SOP Class

Print AE supports the following DIMSE operations for the Film Session SOP Class:

N-CREATE

N-DELETE

Details of the supported attributes and status handling behavior are described in the following subsections.

4.2.1.3.3.5.1 Film Session SOP Class Operations (N-CREATE)

The attributes supplied in an N-CREATE Request are listed in the Table below:

Table 21
Film Session SOP Class N-CREATE Request Attributes

Attribute Name	Tag	VR	Value	Presence of Value	Source
Number of Copies	(2000,0010)	IS	[1, 100]	ALWAYS	CONFIG
Print Priority	(2000,0020)	CS	LOW, MED,HIGH	ALWAYS	CONFIG
Medium Type	(2000,0030)	CS	BLUE FILM, CLEAR FILM, PAPER	ALWAYS	CONFIG
Film Destination	(2000,0040)	CS	MAGAZINE PROCESSOR	ALWAYS	CONFIG

The behavior of Print AE when encountering status codes in a N-CREATE response is summarized in the Table below:

Table 22
Film Session SOP Class N-CREATE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Memory allocation not supported	B60x	The N-CREATE operation is considered successful.
Warning	any warning	xxxx	The N-CREATE operation is considered successful.
Failure	any failure	C60x	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.5.2 Film Session SOP Class Operations (N-DELETE)

The behavior of Print AE when encountering status codes in a N-DELETE response is summarized in the Table below:

Table 23
Printer SOP Class N-DELETE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.

			STANDARD\5,5 STANDARD\5,6 STANDARD\5,7 STANDARD\5,8 STANDARD\6,6 STANDARD\6,7 STANDARD\6,8 STANDARD\6,9 STANDARD\6,10 STANDARD\7,7 STANDARD\7,8 STANDARD\7,9 STANDARD\7,10 STANDARD\8,8 STANDARD\8,9 STANDARD\8,10 LANDSCAPE: STANDARD\1,1 STANDARD\2,1 STANDARD\3,1 STANDARD\1,2 STANDARD\2,2 STANDARD\3,2 STANDARD\4,2 STANDARD\3,3 STANDARD\4,3 STANDARD\5,3 STANDARD\6,3 STANDARD\4,4 STANDARD\5,4 STANDARD\6,4 STANDARD\7,4 STANDARD\8,4 STANDARD\5,5 STANDARD\6,5 STANDARD\7,5		

			STANDARD\8,5 STANDARD\6,6 STANDARD\7,6 STANDARD\8,6 STANDARD\9,6 STANDARD\10,6 STANDARD\7,7 STANDARD\8,7 STANDARD\9,7 STANDARD\10,7 STANDARD\8,8 STANDARD\9,8 STANDARD\10,8		
Referenced Film Session Sequence	(2010,0500)	SQ			
>Referenced SOP Class UID	(0008,1150)	UI	1.2.840.10008.5.1.1.1	ALWAYS	AUTO
>Referenced SOP Instance UID	(0008,1155)	UI	From created Film Session SOP Instance	ALWAYS	AUTO
Film Orientation	(2010,0040)	CS	PORTRAIT or LANDSCAPE	ALWAYS	CONFIG
Film Size ID	(2010,0050)	CS	8INX10IN 8_5INX11IN 10INX12IN 10INX14IN 11INX14IN 11INX17IN 14INX14IN 14INX17IN 24CMX24CM 24CMX30CM A4 A3	ALWAYS	CONFIG
Magnification Type	(2010,0060)	CS	REPLICATE, BILINEAR, CUBIC or NONE	ALWAYS	CONFIG

	Instances (empty page)		
Warning	Image size is larger than Image Box size. The image has been demagnified.	B604H	The N-ACTION operation is considered successful.
Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609H	The N-ACTION operation is considered successful.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image or combined Print Image has been decimated to fit.	B60AH	The N-ACTION operation is considered successful.
Warning	Any other warning	xxxx	The N-ACTION operation is considered successful.
Failure	Unable to create Print Job SOP Instance; print queue is full.	C602	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Image size is larger than Image Box size.	C603	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Combined Print Image Size is larger than Image Box size.	C613	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.
Failure	Any other failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.6.3 Film Session SOP Class Operations (N-DELETE)

The behavior of Print AE when encountering status codes in a N-DELETE response is summarized in the Table below:

Table 27

Printer SOP Class N-DELETE Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The SCP has completed the operation successfully.
Warning	Any warning	xxxx	The N-DELETE operation is considered successful.
Failure	Any other failure	xxxx	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.3.7 SOP Specific Conformance for the Image Box SOP Class

Print AE supports the following DIMSE operations for the Image Box SOP Class:

N-SET

Details of the supported attributes and status handling behavior are described in the following subsections.

4.2.1.3.3.7.1 Image Box SOP Class Operations (N-SET)

The attributes supplied in an N-SET Request are listed in the Table below:

Table 28

Image Box SOP Class N-SET Request Attributes

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Position	(2020,0010)	US	[		

			film sheet		
Basic Color Image Sequence	(2020,0111)	SQ		If the service is configured as RGB	
>Samples Per Pixel	(0028,0002)	US	3	ALWAYS	AUTO
>Photometric Interpretation	(0028,0004)	CS	RGB	ALWAYS	CONFIG
>Planar Configuration	(0028,0006)	US	1	ANAP	AUTO
>Rows	(0028,0010)	US	Depends on film size	ALWAYS	AUTO
>Columns	(0028,0011)	US	Depends on film size	ALWAYS	AUTO
>Pixel Aspect Ratio	(0028,0034)	IS	Set to zero length	VNAP	AUTO
>Bits Allocated	(0028,0100)	US	8	ALWAYS	AUTO
>Bits Stored	(0028,0101)	US	8	ALWAYS	AUTO
>High Bit	(0028,0102)	US	7	ALWAYS	AUTO
>Pixel Representation	(0028,0103)	US	0	ALWAYS	AUTO
>Pixel Data	(7FE0,0010)	OB	Pixels of rendered film sheet	ALWAYS	AUTO

Note 1 If the attribute of Image Display Format is (STANDARD\m, n), num_image is m*n.

The behavior of Print AE when encountering status codes in a N-SET response is summarized in the Table below:

Table 29

Image Box SOP Class N-SET Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	Image print is successful, The status code is logged and the task success is reported to the user via task management.
Warning	Image size is larger than Image Box size. The image has been demagnified.	B604H	The N-SET operation is considered successful.
Warning	Requested Min Density or Max operating range.	B605H	The N-SET operation is considered successful.

Warning	Image size is larger than Image Box size. The image has been cropped to fit.	B609H	The N-SET operation is considered successful.
Warning	Image size or Combined Print Image Size is larger than Image Box size. The image or combined Print Image has been decimated to fit.	B60AH	The N-SET operation is considered successful.
Warning	Any other warning	xxxx	The N-SET operation is considered successful.
Failure	Image size is larger than Image Box size.	C603	The Association is aborted using A-ABORT and the print-job is marked as failed. The status meaning is logged and reported to the user.

4.2.1.3.4 Activity Send Find Request

4.2.1.3.4.1 Description and Sequencing of Activities

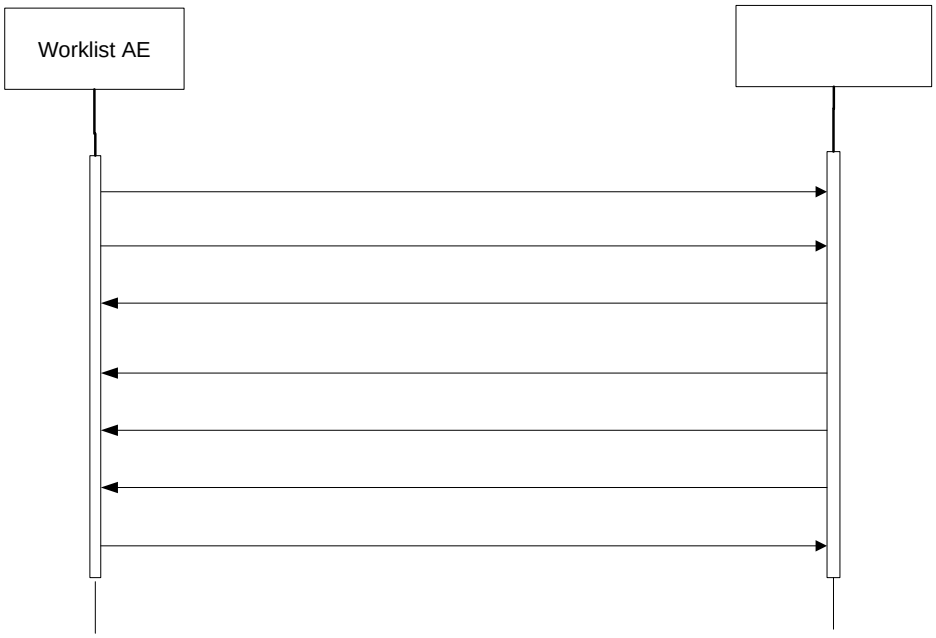

Figure 5

Sequencing of Activity Send FIND Request

A possible sequence of interactions between the Worklist AE and a remote AE (e.g. a system such as a RIS or HIS; or a PACS) is illustrated in the Figure below:

1. The Worklist AE opens an association with the remote AE
2. The Worklist AE sends a C-FIND request to the remote AE containing the Query attributes.
3. The remote AE generates a C-FIND response for the first match.
4. The remote AE generates another C-FIND response for each match.
5. When the process of matching is complete a C-FIND response is sent with a status of Success
6. The C-Find AE closes the association with the remote AE.

4.2.1.3.4.2 Proposed Presentation Contexts

Table 30

Proposed Presentation Contexts for Worklist AE

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Extended Negotiation**
Name	**UID**	**Name**	**UID**		
Modality Worklist Information	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR	1.2.840.10008.1.2.1	SCU	None

Model Find		Little Endian			
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

Worklist AE will propose Presentation Contexts for the SOP Classes listed above. For these SOP Class, Worklist AE will propose multiple Presentation Contexts, one for each of the supported Transfer Syntaxes.

If Worklist AE is offered a choice of Transfer Syntaxes in the accepted Presentation Contexts, it will apply the first encountered to use for the C-FIND operation.

4.2.1.3.4.3 SOP Specific Conformance

Table 31
C_FIND Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior (as SCU)
Refused	Out of resources	A700	The association is aborted using A-ABORT and a notify message is displayed: Some errors happen when query worklist server.
Failed	Identifier Does Not Match SOP Class	A900	
Failed	Unable to process	Cxxx	
Cancel	Matching terminated due to Cancel request	FE00	/
Success	Matching is complete - No final Identifier is supplied.	0000	Patient lists show on the UI
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys.	FF00	/
Pending	Matches are continuing - Warning that one or more Optional Keys were not supported for existence for this Identifier.	FF01	/
*	The Association is aborted using A-ABORT and the query is marked as failed. The status meaning is logged and reported to the user if an interactive query. Any additional error information in the Response will be logged.	Any other status code.	The association is aborted using A-ABORT and a notify message is displayed: Some errors happen when query worklist server.

Worklist AE provides Standard Conformance to the Storage Service Class.

Worklist AE will behave as described in the Table 31 in response to the status returned in the C-FIND response command message.

The behavior of Ultrasound System during communication failure is summarized in the Table below.

Table 32

COMMUNICATION FAILURE BEHAVIOR FOR WORKLIST AE

Exception	Behavior
Timeout	The Association is aborted using A-ABORT and the query marked as failed. The reason is logged and reported to the user if an interactive query.
Association aborted by the SCP or network layers	The query is marked as failed. The reason is logged and reported to the user if an interactive query.

The Table below provides a description of the Ultrasound system Worklist Request Identifier and specifies the attributes that are copied into the images. Unexpected attributes returned in a C-FIND response are ignored.

Requested return attributes not supported by the SCP are set tonull value. Non-matching responses returned by the SCP due to unsupported optional matching keys are ignored. Duplicate entries won t be filter out. No attempt is made to filter out possible duplicate entries.

Table 33

Worklist Request Identifier

ATTRIBUTE	VR	ATTRIBUTE NAME	MATCHING KEYS	RETURN KEYS
Module: Patient Identification Module (M)				
(0010,0010)	PN	Patient's Name	configurable	X (DI)
(0010,0020)	LO	Patient ID	configurable	X(DI)
(0010,1000)	LO	Other Patient IDs		X (DI)
Module: Patient Demographic Module (M)				
(0010,0030)	DA	Patient's Birth Date		X(DI)
(0010,0032)	TM	Patient's Birth Time		X(DI)
(0010,0040)	CS	Patient's Sex		X(DI)
(0010,1020)	DS	Patient's Size		X (DI)
(0010,1030)	DS	Patient's Weight		X (DI)
(0010,2160)	SH	Ethnic Group		X (DI)
(0010,4000)	LT	Patient Comments		X (DI)
(0040,3001)	LO	Confidentiality constraint on patient data		X (DI)

		Description		
Module: Patient Medical Module (M)				
(0010,2000)	LO	Medical Alerts		X (DI)
(0010,2110)	LO	Contrast Allergies		X (DI)
(0010,21B0)	US	History		X (DI)
(0010,21C0)	US	Pregnancy Status		X (DI)
(0010,21D0)	DA	Last Menstrual Date		X (DI)
(0038, 0050)	LO	Special Needs		X (DI)
(0038, 0500)	LO	Patient State		X (DI)
Module: Visit Relationship Module (M)				
(0008,1120)	SQ	Referenced Patient Sequence		X (DI)
Module: Visit Identification Module (M)				
(0038,0010)	LO	Admission ID		X (DI)
Module: Visit Status Module (M)				
(0038,0300)	LO	Current Patient Location		X (DI)
Module: Visit Admission Module (M)				
(0008,1080)	LO	Admitting Diagnosis Description		X (DI)
Module: Scheduled Procedure Step Module (M)				
(0040,0100)	SQ	Scheduled Procedure Step Sequence		X (DI)
>(0008,0060)	CS	Modality	Configurable and the default set to last used value	
>(0032,1070)	LO	Requested Contrast Agent		X (DI)
>(0040,0001)	AE	Scheduled Station AE Title	configurable and the default set to your AE title	X (DI)
>(0040,0002)	DA	Scheduled Procedure Step Start Date	configurable and the date	X(DI)
>(0040,0003)	TM	Scheduled Procedure Step Start Time		X (DI)

>(0040,0004)	DA	Scheduled Procedure Step End Date		X (DI)
>(0040,0005)	TM	Scheduled Procedure Step End Time		X (DI)
>(0040,0006)	PN	Scheduled Performing Physician's Name		X (DI)
>(0040,0007)	LO	Scheduled Procedure Step Description		X(DI)
>(0040,0008)	SQ	Scheduled Protocol Code Sequence		X (DI)
> >(0008,0100)	SH	Code Value		X (DI)
> >(0008,0102)	SH	Coding Scheme Designator		X (DI)
> >(0008,0103)	SH	Coding Scheme Version		X (DI)
> >(0008,0104)	LO	Code Meaning		X (DI)
>(0040,0009)	SH	Scheduled Procedure Step ID		X (DI)
>(0040,0010)	SH	Scheduled Station Name		X (DI)
>(0040,0011)	SH	Scheduled Procedure Step Location		X (DI)
>(0040,0012)	LO	Pre-Medication		X (DI)
> (0040,0020)	CS	Scheduled Procedure Step Status		X (DI)
> (0040,0400)	LT	Comments on the Scheduled Procedure Step		X (DI)
Module: Requested Procedure Module (M)				
(0008,1110)	SQ	Referenced Study Sequence		X (DI)
> (0008,1150)	UI	Referenced SOP Class UID		X (DI)
> (0008,1155)	UI	Referenced SOP Instance UID		X (DI)
(0020,000D)	UI	Study Instance UID		X (DI)
(0032,1060)	LO	Requested Procedure		X (DI)

4.2.1.3.5 Activity Send MPPS Request

4.2.1.3.5.1 Description and Sequencing of Activities

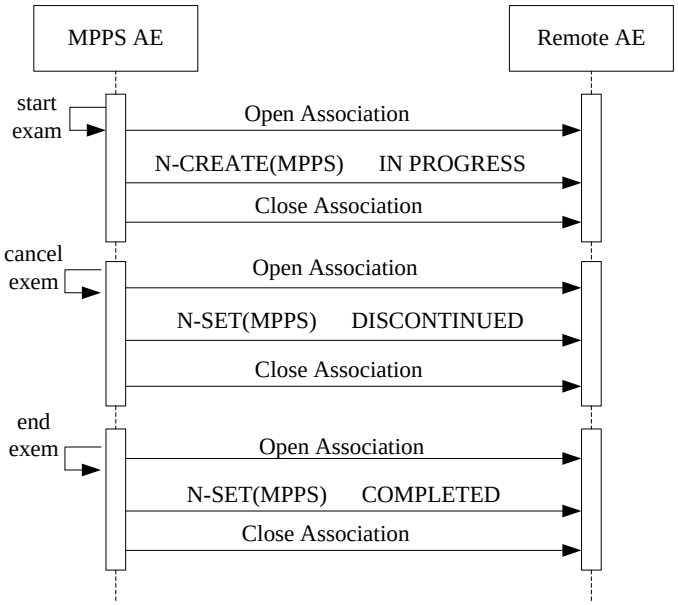

Figure 6

Sequencing of Activity MPPS progress

Note: The Cancel and End Exam commands are mutually exclusive. They are both represented here for illustration purposes only. Actual workflow uses one or the other for a given exam.

For each exam step transfer, an attempt will be made to transmit it to the selected remote AE. If it fails, user can restart the failed task by pressing Retry Button on the DICOM task dialog.

4.2.1.3.5.2 Proposed Presentation Contexts

Table 34

Proposed Presentation Contexts for MPPS AE

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Extended Negotiation**
Name	**UID**	**Name**	**UID**		
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

MPPS-SCU will propose Presentation Contexts for the SOP Classes listed above. For these SOP Class, MPPS-SCU will propose multiple Presentation Contexts, one for each of the supported Transfer Syntaxes.

If MPPS AE is offered a choice of Transfer Syntaxes in the accepted Presentation Contexts, the first encountered will be used for the MPPS AE operation.

4.2.1.3.5.3 SOP Specific Conformance

MPPS AE provides Standard Conformance to the MPPS Service Class.

MPPS-SCU will behave as described in the Table below in response to the status returned in the N-Create or N-Set response command message.

Table 35
MPPS Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior(As scu)
Success	The performed procedure steps are successfully transferred	0000	The N-SET operation is considered successful and the MPPS uid is saved in system.
Warning	The association is aborted using A-ABORT and the transfer is marked as failed. The reason is logged and reported to the user.	B60x	
Failed	The association is aborted using A-ABORT and the transfer job is marked as failed. The reason is logged and reported to the user.	C60x	The association is aborted using A-ABORT and the MPPS uid isn't saved.

Table below provides a description of the MPPS N-CREATE and N-SET request identifiers sent by ultrasound system. Empty cells in the N-CREATE and N-SET columns indicate

Table 36
MPPS N-CREATE / N-SET Request Identifier

Attribute Name	Tag	Req. Type N-CREATE	Req. Type N-SET
Module: Performed Procedure Step Relationship Module (M)			
Referenced Patient Sequence	(0008,1120)	2 (Default is set to null)	Not allowed
	(0010,0010)	2	Not allowed
Patient ID	(0010,0020)	2	Not allowed
	(0010,0030)	2	Not allowed
	(0010,0040)	2	Not allowed

Scheduled Step Attribute Sequence	(0040,0270)	1	Not allowed
>Accession Number	(0008,0050)	2	Not allowed
>Referenced Study Sequence	(0008,1110)	2	Not allowed
>Study Instance UID	(0020,000D)	1	Not allowed
>Requested Procedure Description	(0032,1060)	2	Not allowed
>Scheduled Procedure Step Description	(0040,0007)	2	Not allowed
>Scheduled Protocol Code Sequence	(0040,0008)	2	Not allowed
>Scheduled Procedure Step ID	(0040,0009)	2	Not allowed
>Requested Procedure ID	(0040,1001)	2	Not allowed
Module: Image Acquisition Results Module (M)			
Modality	(0008,0060)	1	Not allowed
Study ID	(0020,0010)	2	Not allowed
Performed Protocol Code Sequence	(0040,0260)	2 (Default is set to null)	3
Performed Series Sequence	(0040,0340)	2	3
>Retrieve AE Title	(0008,0054)	2 (Default is set to null)	2
>Series Description	(0008,103E)	2 (Default is set to null)	2
	(0008,1050)	2	2
	(0008,1070)	2	2
>Referenced Image Sequence	(0008,1140)	2	2
>Protocol Name	(0018,1030)	1	1
>Series Instance UID	(0020,000E)	1	1
>Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	2 (Default is set to null)	2
Module: Billing And Material Management Code Module (M)			
Billing Procedure Step Sequence	(0040,0320)	3	3
Film Consumption Sequence	(0040,0321)	3	3
Billing Supplies and Devices Sequence	(0040,0324)	3	3

Module: Performed Procedure Step Information Module (M)			
Procedure Code Sequence	(0008,1032)	2 (Default is set to null)	3
Performed Station AE Title	(0040,0241)	1	Not allowed
Performed Station Name	(0040,0242)	2 (Default is set to null)	Not allowed
Performed Location	(0040,0243)	2 (Default is set to null)	Not allowed
Performed Procedure Step Start Date	(0040,0244)	1	Not allowed
Performed Procedure Step Start Time	(0040,0245)	1	Not allowed
Performed Procedure Step End Date	(0040,0250)	2 (Default is set to null)	3
Performed Procedure Step End Time	(0040,0251)	2	3
Performed Procedure Step Status	(0040,0252)	1	3
Performed Procedure Step ID	(0040,0253)		

4.2.1.3.6 Activity Query/Retrieve from Remote AE

4.2.1.3.6.1 Description and Sequencing of Activities for SCU

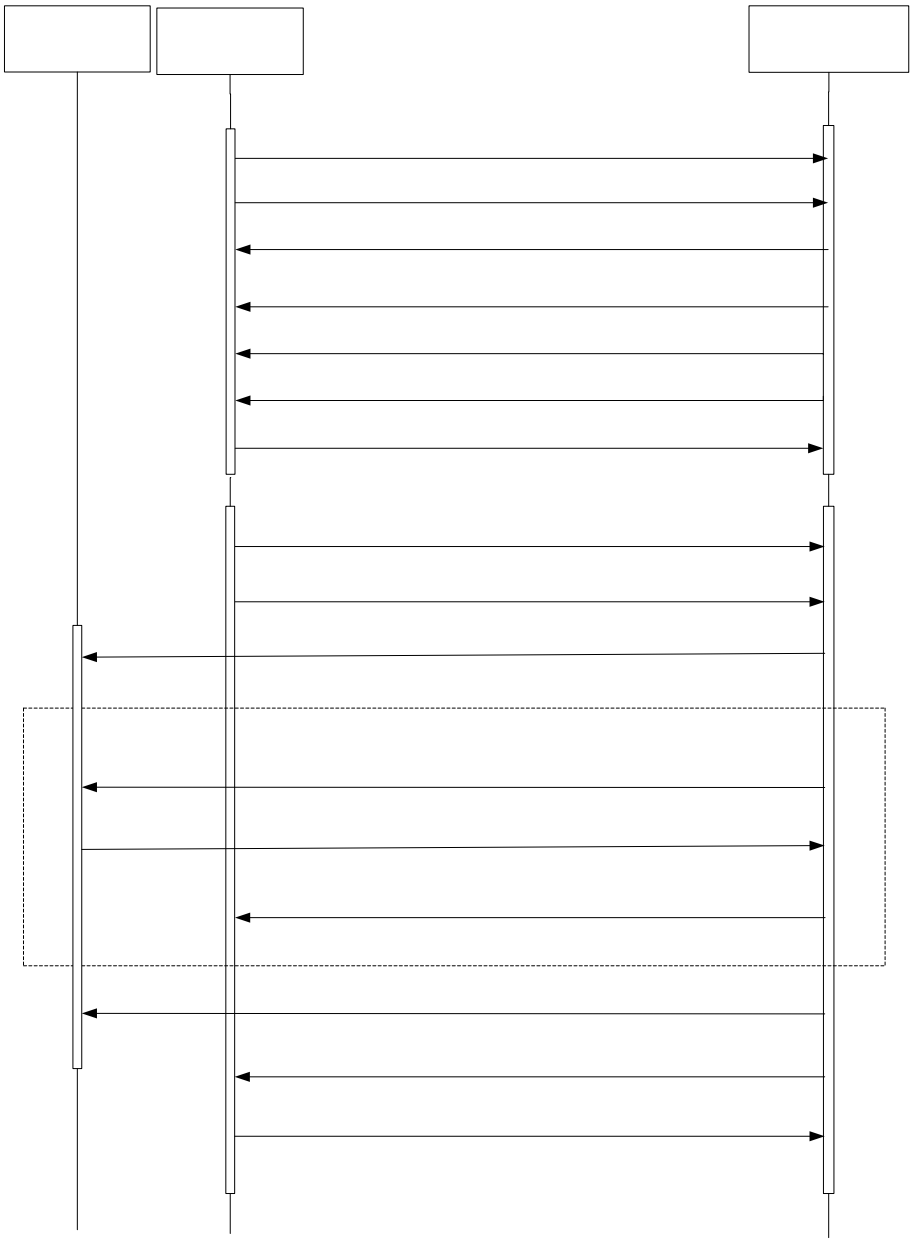

Figure 7

Sequencing of Activity Query/Retrieve progress

The associated Real-World activity is a C-Find request initiated by the user. The user specifies some attributes the system should use to query its database. If the query user successfully establishes an association to the remote AE, it will send a C-Find request (according to the query model) and then the results are returned to the application.

The C-MOVE-RQs are used to retrieve the referenced instances. The Query/Retrieve AE supports the query model Study Root.

4.2.1.3.6.2 Proposed Presentation Contexts

Table 37
Proposed Presentation Contexts for Query/Retrieve AE

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name	UID		
Study Root Query/Retrieve Information Model - Find	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None
Study Root Query/Retrieve Information Model - Move	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

4.2.1.3.6.3 SOP Specific Conformance

The ultrasound system provides Standard Conformance to the DICOM Query/Retrieve Class.

4.2.1.3.6.3.1 Response Status

Query/Retrieve AE will behave as described in the Table below in response to the status returned in the C-Find response command message.

Table 38
C-Find Response Status Handling Behavior

Service Status	Meaning	Protocol Codes	Related Fields	Behavior (as SCU)
Refused	Refused Out of Resources	A700	(0000,0902)	The association is aborted using A-ABORT and a notify message is displayed: The remote server error.
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)	
	Unable to process	CXXX	(0000,0901) (0000,0902)	
Canceling	Matching terminated due to Cancel request	FE00	None	
Success	Matching is complete - No	0000	None	Patient lists show on

	final Identifier is supplied			the UI
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier	/
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier	/

The ultrasound system supports the following query levels:

Study

The Query/Retrieve AE interprets following status codes.

Table 39

C-Move Response Status Handling Behavior

Service Status	Meaning	Protocol Codes	Related Fields	Behavior (as SCU)
Refused	Refused Out of Resources	A700	(0000,0902)	The association is aborted using A-ABORT and a notify message is displayed: The remote server error.
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)	
	Unable to process	CXXX	(0000,0901) (0000,0902)	
Canceling	Matching terminated due to Cancel request	FE00	None	
Success	Matching is complete - No final Identifier is supplied	0000	None	Image retrieve is successful, Patient lists show on the UI
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier	/
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier	/

4.2.1.3.6.3.2 Study Root Query/Retrieve Attributes

4.2.1.3.6.3.3 Supported Matching

Following are the types of matching that can be request by the implementation:

- Single Value matching
- Universal Matching
- Wild Card Matching
- Range of date, Range of Time

The user can filter the downloaded C-FIND result, to view a limited set of the result.

4.2.1.3.6.3.4 Study Level

This section defines the keys at the Study Level of the Study Root Query/Retrieve Information Model that are supported by this implementation.

Table 40

STUDY LEVEL ATTRIBUTES

MODULE: STUDY ROOT INFORMATION MODEL (M)					
Attribute	**VR**	**Type**	**Attribute Name**	**Value**	**Matching keys**
Module: Study Root Information Model (M)					
(0008,0020)	DA	R	Study Date		DA(SK)
(0008,0030)	TM	R	Study Time		N
(0010,0010)	PN	R	Patient's Name		*(SK)
(0010,0020)	LO	R	Patient ID		S(SK)

(0010,2160)	SH	O	Ethnic Group		N
(0010,2180)	SH	O	Occupation		N
(0010,21B0)	LT	O	Additional Patient History		N
(0010,4000)	LT	O	Patient Comments		N
(0020,1070)	IS	O	Other Study Numbers		N
(0020,1200)	IS	O	Number of Patient Related Studies		N
(0020,1202)	IS	O	Number of Patient Related Series		N
(0020,1204)	IS	O	Number of Patient Related Instances		N
(0020,1206)	IS	O	Number of Study Related Series		N
(0020,1208)	IS	O	Number of Study Related Instances		N
(4008,010C)	PN	O	Interpretation Author		N
Module: Additional Attributes Module (O)					
(0008,0062)	UN	O	SOP Classes in Study		N

4.2.1.3.6.3.5 Series Level Attributes

Table 41

SERIES LEVEL ATTRIBUTES

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE	MATCHINGKEYS
Module: Study Root Information Model (M)					
(0020,000D)	UI	U	Study Instance UID		S
(0020,000E)	UI	U	Series Instance UID		N
(0008,0060)	CS	R	Modality		N
(0020,0011)	IS	R	Series Number		N
(0020,1209)	IS	O	Number of Series Related Instances		N
Module: Additional Attributes Module (O)					
(0008,0021)	DA	O	Series Date		N
(0008,0031)	TM	O	Series Time		N

4.2.1.3.6.3.6 Composite Object Instance Level

Table 42

COMPOSITE OBJECT INSTANCE LEVEL ATTRIBUTES

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE	MATCHINGKEYS
Module: Study Root Information Model (M)					
(0020,000D)	UI	U	Study Instance UID		S
(0020,000E)	UI	U	Series Instance UID		S
(0008,0018)	UI	U	SOP Instance UID		N
(0020,0013)	IS	R	Instance Number		N
Module: Additional Attributes Module (O)					
(0008,0016)	UI	O	SOP Class UID		N
(0008,001A)	UI	O	Related General SOP Class UID		N
(0008,3001)	SQ	O	Alternate Representation Sequence		N
>(0008,1150)	UI	O	Referenced SOP Class UID		N
>(0008,1155)	UI	O	Referenced SOP Instance UID		N
>(0020,000E)	UI	O	Series Instance UID		N
>(0040,A170)	SQ	O	Purpose of Reference Code Sequence		N
>>(0008,0100)	SH	O	Code Value		N
>>(0008,0102)	SH	O	Coding Scheme Designator		N
>>(0008,0103)	SH	O	Coding Scheme Version		N
>>(0008,0104)	LO	O	Code Meaning		N
(0040,A043)	SQ	O	Concept Name Code Sequence		N
>(0008,0100)	SH	O	Code Value		N
>(0008,0102)	SH	O	Coding Scheme Designator		N
>(0008,0103)	SH	O	Coding Scheme Version		N
>(0008,0104)	LO	O	Code Meaning		N
(0040,A504)	SQ	O	Content Template Sequence		N
>(0008,0105)	CS	O	Mapping Resource		N
>(0040,DB00)	CS	O	Template Identifier		N

4.2.1.4 Association Acceptance Policy

4.2.1.4.1 Activity Receive Echo Request

4.2.1.4.1.1 Description and Sequencing of Activities

The Verification AE (as SCP) accepts associations only if Presentation Contexts hanve been validated If Verification AE (as SCP) receives an echo (C-ECHO) request then the response will be sent over the same association used to send the C-ECHO-RQ.

Table 44

Proposed Presentation Contexts for Storage

PROPOSED PRESENTATION CONTEXTS					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name**	**UID**		
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCP	None
US Multiframe Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCP	None
Secondary	1.2.840.100	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None

Capture Image Storage	08.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		JPEG Lossy, Baseline Sequential with Huffman Coding (Process 1)	1.2.840.10008.1.2.4.50	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14 [Selection Value 1])	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		JPEG 2000 Image Compression (Lossless Only)	1.2.840.10008.1.2.4.90	SCP	None
		JPEG 2000 Image Compression	1.2.840.10008.1.2.4.91	SCP	None
Comprehensive Structured Report Storage					

4.2.1.4.3.2 Accepted Presentation Contexts

The Storage Commitment AE will accept Presentation Contexts as shown in the Table below.

Table 45

Acceptable Presentation Contexts for

Activity Receive Storage Commitment Response

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	SCU	None

The Storage Commitment AE will only accept the SCU role within a Presentation Context for the Storage Commitment Push Model SOP Class.

4.2.1.4.3.3 SOP Specific Conformance

4.2.1.4.3.3.1 Storage Commitment Operations (N-ACTION)

The Storage Commitment AE will issue a storage commitment request after the successful transfer of an end exam storage task .

The behavior of Storage Commitment AE when receiving N-Action response status codes is summarized in the Table below:

Table 46

Storage Commitment N-ACTION Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Success	Success	0000	The request for storage commitment is considered successfully sent. The ultrasound system waits for the N-EVENT-REPORT in background.
*	*	Any other status code.	The request for storage commitment is failed.

The behavior of Storage Commitment AE during communication failure is summarized in the Table below:

Table 47

Storage Commitment Communication Failure Behavior

Exception	Behavior
Timeout	The Association is aborted using A-ABORT and the send job is marked as failed.
Association aborted by the SCP or network layers	The send job is marked as failed.

4.2.1.4.3.3.2 Storage Commitment Tags (N-ACTION)

The Storage Commitment AE will request storage commitment using the following tags.

NOTE: Storage Commitment may only be automatically requested upon successful completion of an end exam storage task.

Table 48

Storage Commitment N-Action-Request Message Contents

Action Type Name	Event Type ID	Attribute	Tag
N-ACTION-RQ (M)	1	Requested SOP Class UID	(0000,0003)
		Requested SOP Instance UID	(0000,1001)
Module: Additional Attributes Module (O)	3	Instance Creation Date	(0008,0012)
		Instance Creation Time	(0008,0013)
Request Storage Commitment	1	Transaction UID	(0008,1195)
		Referenced SOP Sequence	(0008,1199)
		>Referenced SOP Class UID	(0008,1150)
		>Referenced SOP Instance UID	(0008,1155)

4.2.1.4.3.3.3 Storage Commitment Notifications (N-EVENT-REPORT)

The reasons for returning specific status codes in a N-EVENT-REPORT response are summarized in the Table below.

The Error Code represent service status should be sent with one of the values as below.

Table 49

Storage Commitment N-EVENT-REPORT Response Status Reasons

Service Status	Further Meaning	Error Code
Success	N-EVENT-REPORT message operate success.	0000
Failed	N-EVENT-REPORT message operate failed.	0110

4.2.1.4.3.3.4 Storage Commitment Tags (N-EVENT- REPORT)

Tags supported for receiving an N-Event-Report message are listed as below.

Table 50

Storage Commitment N-Event-Report Message Contents

EVENT TYPE NAME	EVENT TYPE ID	ATTRIBUTE	TAG	REQUIREMENT TYPE SCP
Storage Commitment Request Successful	1	Transaction UID	(0008,1195)	1
		Referenced SOP Sequence	(0008,1199)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1
Storage Commitment Request Complete Failures Exist	2	Transaction UID	(0008,1195)	1
		Referenced SOP Sequence	(0008,1199)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1
		Failed SOP Sequence	(0008,1198)	1
		>Referenced SOP Class UID	(0008,1150)	1
		>Referenced SOP Instance UID	(0008,1155)	1
		>Failure Reason	(0008,1197)	1

4.3 Network Interface

4.3.1 Supported Communications Stacks

Modality DICOM AEs provide DICOM 3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

4.3.2 TCP/IP Stack

Modality DICOM AEs inherit their TCP/IP stack from the Linux Operating System upon which they execute.

4.3.3 Physical Network Interface

Modality supports a single network interface. One of the following physical network interfaces will be available depending on installed hardware options:

Table 51

Supported Physical Network Interfaces

Ethernet 100baseT
Ethernet 10baseT

Print:

- Device, Service name, AE Title and Port .
- Timeout.
- Maximum retries. (default value is 3)
- Interval Time (In this version, this parameter is not usable.)
- Media Type: PAPER, CLEAR FILM, or BLUE FILM
- Film Size:
  - 8INX10IN
  - 8_5INX11IN
  - 10INX12IN
  - 10INX14IN
  - 11INX14IN
  - 11INX17IN
  - 14INX14IN
  - 14INX17IN
  - 24CMX24CM
  - 24CMX30CM
  - A4
  - A3
- Copies:1-100
- Max Density: 0-65535
- Min Density:0-65535
- Settings: RGB or MONOCHROME2
- Display Format:
  - ✧ PORTRAIT:
    - STANDARD\1,1
    - STANDARD\1,2
    - STANDARD\1,3
    - STANDARD\2,1
    - STANDARD\2,2
    - STANDARD\2,3
    - STANDARD\2,4
    - STANDARD\3,3
    - STANDARD\3,4
    - STANDARD\3,5
    - STANDARD\3,6

Mindray DP-50 Series Digital Ultrasonic Diagnostic Imaging System

STANDARD\7,4
STANDARD\8,4
STANDARD\5,5
STANDARD\6,5
STANDARD\7,5
STANDARD\8, 5
STANDARD\6,6
STANDARD\7,6
STANDARD\8,6
STANDARD\9,6
STANDARD\10,6
STANDARD\7,7
STANDARD\8,7
STANDARD\9,7
STANDARD\10,7
STANDARD\8,8
STANDARD\9,8
STANDARD\10,8

- Destination: MAGAZINE or PROCESSOR
- Film Orientation: LANDSCAPE or PORTRAIT
- Priority: HIGH, MED, or LOW
- Configuration Info
- Magnification Type: NONE, CUBIC, REPLICATE, or BILINEAR
- Trim: Yes/Not
- Default Status (Y/N)

WORKLIST:

- Device, Service name, AE Title and Port .
- Timeout.
- Maximum retries, Interval Time (In this version, these two parameters are not usable.)
- Default Status (Y/N)

MPPS:

- Device, Service name, AE Title and Port.
- Timeout,
- Maximum retries (default value is 3)
- Interval Time (In this version, this parameter is not usable.)

- Default Status (Y/N)

Storage Commitment:

- Device, Service name, AE Title and Port.
- Timeout.
- Maximum retries, Interval Time (In this version, these tw-4( )]8(t)5(h)11(e)1124.76 702.43 Tm[(o)11(r)-7(t

5 Media Storage

5.1 Implementation Model

5.1.1 Application Data Flow

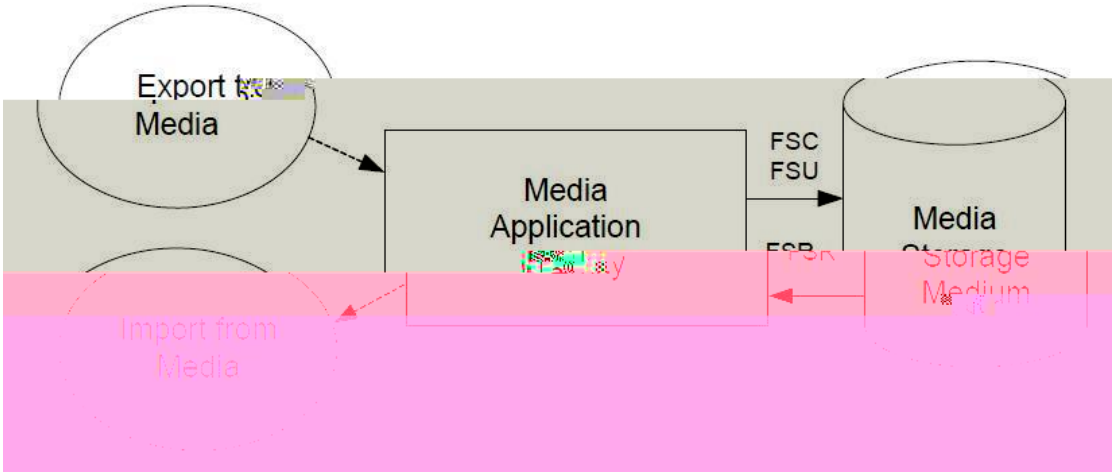

Figure 9

Application Data Flow Diagram for Media Storage

The Media Application Entity exports Images and Structured Reports to a removable storage medium. It is associated with the local real- Backup configured export selection parameters for selected Structured Reports).

5.1.2

5.1.2.1 Functional Definition of Media Application Entity

images to the Media Application Entity. The contents of each export job will be written to the selected media destination. The size of the selected media is used to determine and display the number of media required for the export. When a device is filled to capacity, the system will prompt the user for addition media and continue.

5.1.3 Sequencing of Real-World Activities

At least one image must exist and be selected before the Media Application Entity can be invoked. The operator can insert new media at any time. The Media Application Entity will wait indefinitely for media to be inserted before starting to write to the device.

5.1.4 File Meta Information Options

The implementation information written to the File Meta Header in each file is:

Table 52

5.2.1.2.2 Activity-FSR-Import exams

When system user presents the directory of the media, presses Restore button and the selected exams are transferred from the media to the system for review. Objects transferred to the system retain their original SOP Instance UIDs.

The Media Application Entity acts as an FSR using the interchange option when requested to import SOP Instances from media to the local database.

5.2.1.2.3 Activity-FSU-Export exams

The system user sele

already contains data. The DICOMDIR is updated allowing access to original and new data.

The Media Application Entity acts as an FSU using the interchange option when requested to export SOP Instances from the local database to media upon which DICOM data already resides.

5.2.1.2.3.1 Media Storage Application Profiles

See Table 53 for supported Application Profiles.

5.2.1.2.3.1.1 Options

The Media Application Entity supports the SOP Classes and Transfer Syntaxes listed in the Table below:

Table 54
IODs, SOP Classes and Transfer Syntaxes

Information Object Definition	SOP Class UID	Transfer Syntax	Transfer Syntax UID
DICOM Media Storage Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian	1.2.840.10008.1.2.1
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian	1.2.840.10008.1.2.1
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian	1.2.840.10008.1.2.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian	1.2.840.10008.1.2.1

Table 57

Study Directory Record

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
(0004,1430)	CS	1	Directory Record Type	STUDY
(0008,0020)	DA	1	Study Date	AUTO
(0008,0030)	TM	1	Study Time	AUTO
(0020,0010)	SH	1	Study ID	AUTO
(0020,000D)	UI	1C	Study Instance UID	AUTO
(0008,0050)	SH	2	Accession Number	MWL/USER
(0008,1030)	LO	2	Study Description	If it is a scheduled exam, the value is mapped from Scheduled Procedure Step Description; If not, USER
(0008,0090)	PN		Referring Physician's Name	MWL/USER

Table 58

Series Directory Record

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
(0004,1430)	CS	1	Directory Record Type	SERIES
(0008,0060)	CS	1	Modality	US
(0020,000E)	UI	1	Series Instance UID	AUTO
(0020,0011)	IS	1	Series Number	AUTO
(0008,0021)	DA	3	Series Date	AUTO
(0008,0031)	TM	3	Series Time	AUTO
(0008,103e)	LO		Series Description	If it is a scheduled exam, the value is mapped from Scheduled Procedure Step Description; If not, same as the value of Study Description
(0008,1050)	PN		Performing Physician's Name	MWL/USER

Table 59

Image Directory Record

ATTRIBUTE	VR	TYPE	ATTRIBUTE NAME	VALUE(S) AND COMMENTS
(0004,1430)	CS	1	Directory Record Type	IMAGE
(0004,1500)	CS	1C	Referenced File ID	AUTO
(0004,1510)	UI	1C	Referenced SOP Class UID in File	AUTO
(0004,1511)	UI	1C	Referenced SOP Instance UID in File	AUTO
(0004,1512)	UI	1C	Referenced Transfer Syntax UID in File	AUTO
(0020,0013)	IS	1	Instance Number	AUTO
(0028,0008)	IS	3	Number of Frames	AUTO(Only used for mutil-frame image)

5.4 Augmented and Private Application Profiles

No augmented/private profile is supported.

5.5 Media Configuration

None.

6 SUPPORT OF CHARACTER SETS

In addition to the default character repertoire, the Defined Terms for Specific Character Set in Table 60 are supported:

Table 60

Supported Specific Character Set Defined Terms

Character Set Description	Defined Term	System Language
ISO 8859-1	ISO_IR 100	English, French, German, Italian, Portuguese, Spanish, Finnish, Danish, Icelandic, Norwegian, Swedish
ISO 8859-5	ISO_IR 144	Russian
ISO-8859-2	ISO_IR 101	Polish, Czech
ISO-8859-9	ISO_IR 148	Turkish
Chinese	GB18030	Chinese

If the system language is configured for one of above languages, the corresponding Character Set will be used automatically. Whether or not characters are displayed correctly depends on the operating system. For example, if the system is configured for Turkish, the characters of Turkish could display correctly.

7 SECURITY

7.1 Security Profiles

None supported.

7.2 Association level security

None supported.

Any Calling AE Titles and/or IP addresses may open an Association.

7.3 Application level security

None supported.

8.5 Standard extended/specialized/private sop Classes

None.

8.6 Private Transfer Syntaxes

None.

The DP-50 Vet don t support SR.

A. Appendix : OB GYN structured reporting template

None supported SR in the use of animal.

This appendix lists the DICOM Structured Report (SR) mappings used in the Obstetric and Gynecologic Structured Reports of ultrasound system SR files.

The mappings are organized in a manner similar to the DICOM SR Templates as described in PS 3.16 of the DICOM Standard. The OB-GYN Report mappings follow the DICOM SR Template TID 5000: OB-GYN Ultrasound Procedure Report, except where noted.

All private code values use the Coding Scheme Designator "MRUS".

A.1. TID (300) Measurement

This Template provides a general structure for a numeric measurement, together with evaluations of its normality and/or significance, and the inference source(s) for its value.

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			NUM	$Measurement			Units = $Units
2	>	HAS CONCEPT MOD	CODE	EV (G-C036, SRT, "Measurement Method")			$Method
3	>	HAS CONCEPT MOD	CODE	EV (121401, DCM, "Derivation")			$Derivation
4	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT, "Finding Site")			$TargetSite
5	>>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT, "Laterality")			DCID (244) Laterality
6	>	HAS PROPERTIES	CODE	EV (121404, DCM, "Selection Status")			
7	>	INFERRED FROM	CODE	DCID (228) Equation or Table			
8	>>	HAS PROPERTIES	NUM				

A.2. TID 1008 Subject Context, Fetus

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			PNAME	EV (121036,DCM,			
2			UIDREF	EV (121028,DCM,			
3			TEXT	EV (121030,DCM,			
4			TEXT	EV (11951-1,LN,			
5			NUM	EV (11878-6,LN, "Number of			

A.3. TID (5000) OB-GYN Ultrasound Procedure Report

This is the template for the root of the content tree for the OB-GYN ultrasound procedure report.

NO	**NL**	**Relation with Parent**	**Value Type**	**Concept Name**	**Used in MODALITY**	**Condition**	**Value Set Constraint**
1			CONTAINER	EV (125000, -GYN Ultrasound Procedure			
2	>	HAS CONCEPT MOD	INCLUDE	DTID (1204) Language of Content Item and Descendants			
3	>	HAS OBS CONTEXT	INCLUDE	DTID (1001) Observation Context			
4	>	CONTAINS	INCLUDE	DTID (5001) Patient Characteristics			
5	>	CONTAINS	CONTAINER	DT (111028,			

6	>>	CONTAINS	IMAGE	No purpose of reference			
7	>	CONTAINS	INCLUDE	DTID (5002) OB-GYN Procedure Summary Section			
8	>	CONTAINS	INCLUDE	DTID (5004) Fetal Biometry Ratio Section			
9	>	CONTAINS	INCLUDE	DTID (5005) Fetal Biometry Section			
10	>	CONTAINS	INCLUDE	DTID (5006) Long Bones Section			
11	>	CONTAINS	INCLUDE	DTID (5007) Fetal Cranium Section			
12	>	CONTAINS	INCLUDE	DTID (5009) Fetal Biophysical Profile Section			
13	>	CONTAINS	INCLUDE	DTID (5011) Early Gestation Section			
14	>	CONTAINS	INCLUDE	DTID (5010) Amniotic Sac Section			
15	>	CONTAINS	INCLUDE	DTID (5015) Pelvis and Uterus Section			
16	>	CONTAINS	INCLUDE	DTID (5012) Ovaries Section			
17	>	CONTAINS	INCLUDE	DTID (5013) Follicles Section			$Laterality = EV (G- $Number = EV (11879- of follicles in left
18	>	CONTAINS	INCLUDE	DTID (5013) Follicles Section			$Laterality = EV (G- $Number = EV (11880- of follicles in right

19	>	CONTAINS	CONTAINER	EV (121070,			
20	>>	HAS CONCEPT MOD	CODE	EV (G-C0E3, Finding			EV (T-F6800, SRT,
21	>>	CONTAINS	INCLUDE	DTID (5025) OB-GYN Fetal Vascular Measurement Group			$AnatomyGroup = DCID (12141) Fetal Vasculature
22	>	CONTAINS	CONTAINER	EV (121070,			
23	>>	HAS CONCEPT MOD	CODE	EV (G-C0E3,			EV (T-D6007, SRT,
24	>>	CONTAINS	INCLUDE	DTID (5026) OB-GYN Pelvic Vascular Measurement Group			$AnatomyGroup = DCID (12140) Pelvic Vasculature Anatomical Location
25	>	CONTAINS	INCLUDE	DTID (SELFTMP-1)			

A.4. TID (SELFTMP-1) Fetal Cardiac Measurement Group

This is a private template referenced by TID (5000).

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	EV(T0001,MRUS,Fetel Cardiac)			
2	>	HAS OBS CONTEXT	INCLUDE	DTID (1008) Subject Context, Fetus			
3	>	CONTAINS	INCLUDE	DTID (SELFTMP-2) Fetal ZSCORE			$MeasType = DCID (SELFCID-1) Fetal Z-Score $Derivation = DCID (3627) Measurement Type

A.5. TID (SELFTMP-2) Fetal ZScore

This is a private template referenced by TID (5000).

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	INCLUDE	DTID (300) Measurement			
2		CONTAINS	NUM	EV (C12017-1, MRUS, -Score by Femur			calculated by $MeasType and Femur Length
3		CONTAINS	NUM	EV (C12017-2, MRUS, -Score by Biparietal			calculated by $MeasType and Biparietal Diameter
4		CONTAINS	NUM	EV (C12017-3, MRUS, -Score by Clinical			calculated by $MeasType and Clinical Gestational Age

A.6. TID (1001) OBSERVATION CONTEXT

This template specifies attributes of observation context that may be defined, extended or replaced at any location in the SR tree.

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1	>	HAS OBS CONTEXT	CODE	EV (121005,DCM,			(121006,DCM,
2	>	HAS OBS CONTEXT	PNAME	EV (121008,DCM,			Operator from Info
3	>	HAS OBS CONTEXT	TEXT	EV (121009,DCM,			Institution Name (0008,0080) of the General Equipment Module
4	>	HAS OBS CONTEXT	CODE	EV (121010,DCM, Role in the			(121093, DCM, "Sonographer")
5	>	HAS OBS CONTEXT	CODE	EV (121024, DCM,			(121025, DCM,
6	>	HAS OBS CONTEXT	PNAME	EV (121029,DCM,			Name (0010,0010) in Patient Module

7	>	HAS OBS CONTEXT	DATE	EV (121031,DCM,			Birth Date (0010,0030) in Patient Module
8	>	HAS OBS CONTEXT	CODE	EV (121032,DCM,			value equivalent to (0010,0040) in Patient Module
9	>	HAS OBS CONTEXT	NUM	EV (121033,DCM,			Age (0010,1010) in Patient Study Module

A.7. TID (5001) OB-GYN Patient Characteristics

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	EV (121118, DCM,			
2	>	CONTAINS	TEXT	EV (121106, DCM,			
3	>	CONTAINS	NUM	EV (8302-2, LN,			
4	>	CONTAINS	NUM	EV (29463-7, LN,			
5	>	CONTAINS	NUM	EV (11996-6, LN,			from info
6	>	CONTAINS	NUM	EV (11977-6, LN,			from info
7	>	CONTAINS	NUM	EV (11612-9, LN,			from info
8	>	CONTAINS	NUM	EV (33065-4, LN,			from info(Ectopic)

A.8. TID (5002) OB-GYN Procedure Summary

NO	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (121111, DCM,			

2	>	CONTAINS	DATE	11778-8, LN, "EDD"			from info
3	>	CONTAINS	DATE	(11779-6, LN, "EDD from LMP")			from info
4	>	CONTAINS	DATE	(11781-2, LN, "EDD from average ultrasound age")			
5	>	CONTAINS	DATE	11780-4, LN, "EDD from ovulation date"			from info
6	>	CONTAINS	DATE	(11955-2, LN, "LMP"			from info
7	>	CONTAINS	DATE	33066-2, LN, "Estimated LMP by EDD"			from info
8	>	CONTAINS	DATE	11976-8, LN, "Ovulation date"			from info
9	>	CONTAINS	DATE	(I12003-01, MRUS, "IVF")			from info
10	>	CONTAINS	DATE	(C12003-01, MRUS, "EDD from IVF")			from info
11	>	CONTAINS	DATE	(I12003-02, MRUS, "PRV")			from info
12	>	CONTAINS	DATE	(C12003-02, MRUS, "EDD from PRV")			from info
13	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11886-9, LN, "Gestational Age by ovulation date")
14	>	CONTAINS	TEXT	EV (121106, DCM, Comment)			from info
15	>	CONTAINS	TEXT	(I12101-01, MRUS, "Primary Indications")			from info
16	>	CONTAINS	TEXT	(I12101-02, MRUS, "Secondary Indications")			from info
17	>	CONTAINS	TEXT	(I12101-03, MRUS, "CPT4 Code")			from info
18	>	CONTAINS	TEXT	(I12101-04,			from info

21	>	CONTAINS	TEXT	(121071, DCM, "Findings")			report interface Findings
22	>>		INCLUDE	DTID (320) Image or Spatial Coordinates			
23	>	CONTAINS	INCLUDE	BTID (5003) OB-GYN Fetus Summary			

A.9. TID (5003) OB-GYN Fetus Summary

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125008, DCM,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,"Fetus			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (18185-9, LN, "Gestational Age")
5	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11888-5, LN, " Composite Ultrasound Age")
6	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11885-1, LN, "Gestational Age
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11727-5, LN, "Estimated
8	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11767-1, LN, "EFW percentile rank")
9	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11948-7, LN, " Fetal Heart Rate")

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
10	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-01, MRUS, "Gestational Age by IVF")
11	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (I12019-01, MRUS, "GA of Previous Exam")
12	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-02, MRUS, "Gestational Age by PRV")
13	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-03, MRUS, "Gestational Age by EDD")
14	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-4, MRUS, "Gestational Age by EFW")
15	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (C12019-4, MRUS, "Gestational Age by mean Gestational Sac Diameter")
16	>	CONTAINS	INCLUDE	FINDING_1			
17	>	CONTAINS	INCLUDE	FINDING_2			
18	>	CONTAINS	INCLUDE	FINDING_3			
19	>	CONTAINS	INCLUDE	FINDING_4			
20	>	CONTAINS	INCLUDE	FINDING_5			
21	>	CONTAINS	INCLUDE	FINDING_6			
22	>	CONTAINS	INCLUDE	FINDING_7			

A.10. TID (FINDING_1) Fetal Description

This is a private template referenced by TID (5003).

NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint

NL	Rel with Parent	VT	Concept Name

A.11. TID (FINDING_2) Fetus Limbs

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG4031-03,MRUS,"Fetus Limbs")			
2	>	CONTAINS	TEXT	(FG4031-04,MRUS,"Upper Extremities")			
3	>	CONTAINS	TEXT	(FG4031-05,MRUS,"Lower Extremities")			

A.12. TID (FINDING_3) Fetal Cardiology

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG4031-06,MRUS,"Fetal Cardiology")			
2	>	CONTAINS	TEXT	(FG12239-01,MRUS,"Cardiac Activity")			
3	>	CONTAINS	TEXT	(FG4031-07,MRUS,"4C HEART")			
4	>	CONTAINS	TEXT	(T-42000,SNM3,"Aorta")			
5	>	CONTAINS	TEXT	(T-44000,SNM3,Pulmonary Artery)			
6	>	CONTAINS	TEXT	(FG3010-01,MRUS,"ARCH")			
7	>	CONTAINS	TEXT	(FG3010-03,MRUS," Decrease ARCH ")			

A.13. TID (FINDING_4) Fetal Brain

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG4030-01,MRUS,"Fetal Brain")			
2	>	CONTAINS	TEXT	(FG4030-02,MRUS,"Lateral Ventricles")			
3	>	CONTAINS	TEXT	(11860-4,LN,"Cisterna Magna")			
4	>	CONTAINS	TEXT	(T-A600A,SNM3,"Cerebellum")			
5	>	CONTAINS	TEXT	(FG4030-03,MRUS,"CSP")			

A.14. TID (FINDING_5) Spine

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(T-11500,SRT,"Spine")			
2	>	CONTAINS	TEXT	(T-11501,SNM3,"Cervical Spine")			
3	>	CONTAINS	TEXT	(T-11502,SNM3,"Thoracic Spine")			
4	>	CONTAINS	TEXT	(T-11503,SNM3,"Lumbar Spine")			
5	>	CONTAINS	TEXT	(FG4031-08,MRUS,"Sacral Spine")			

A.15. TID (FINDING_6) Fetal Environment

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG12019-03,MRUS,"Fetal Environment")			
2	>	CONTAINS	TEXT	(FG12011-01,MRUS,"Placental Location")			

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
3	>	CONTAINS	TEXT	(FG12011-02,MRUS,"Amniotic Fluid")			
4	>	CONTAINS	TEXT	(FG12011-03,MRUS,"Placental Grade")			

A.16. TID (FINDING_7) Maternal Description

This is a private template referenced by TID (5003).

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1		CONTAINS	CONTAINER	(FG6088-01,MRUS,"Maternal Description")			
2	>	CONTAINS	CONTAINER	(FG12011-03,MRUS,"Adnexa")			
3	>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
4	>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
5	>	CONTAINS	CONTAINER	(T-87000,SRT,"Ovary")			
6	>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
7	>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
8	>	CONTAINS	CONTAINER	(T-71000,SRT,Kidney)			
9	>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
10	>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
11	>	CONTAINS	TEXT	(T-83200,SRT,Cervix)			

A.17. TID (5004)Fetal Biometry Ratio Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125001, DCM,			

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
2	>	HAS OBS CONTEXT	INCLUDE	EV (11951-1, LN, "Fetus I			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN,			
4	>	CONTAINS	NUM	11947-9, LN, "HC/AC"			
5	>	CONTAINS	NUM	11871-1, LN, "FL/AC"			
6	>	CONTAINS	NUM	11872-9, LN, "FL/BPD"			
7	>	CONTAINS	NUM	(11823-2, LN, "Cephalic Index")			
8	>	CONTAINS	NUM	(11873-7, LN, "FL/HC")			
9	>	CONTAINS	NUM	(C12004-01, MRUS, HrtC/TC)			
10	>	CONTAINS	NUM	(C12004-02, MRUS, "TCD/AC")			
11	>	CONTAINS	NUM	(C12004-03, MRUS, LVW/HW)			
12	>	CONTAINS	NUM	(C12004-04, MRUS, "Cephalic Index by HC")			

A.18. TID (5005) Fetal Biometry Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125002,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN,			
4	>	CONTAINS	INCLUDE	DTID (5008) Fetal Biometry Group			$BiometryType = MemberOf

							{DCID (12005) Fetal Biometry Measurements}

A.19. TID (5006) Fetal Long Bones Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125003,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (5008) Fetal Biometry Group			$BiometryType = MemberOf {DCID (12006) Fetal Long Bones Biometry Measurements}

A.20. TID (5007) Fetal Cranium Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125004,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (5008) Fetal Biometry Group			$BiometryType = MemberOf

							{DCID (12007) Fetal Cranium}

A.21. TID (5008) Fetal Biometry Group

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT(125005,			
2	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $BiometryType $Derivation = DCID (3627) Measurement Type
3	>	CONTAINS	NUM	EV (18185-9,			Units= EV (d,UCUM, days)
4	>>	INFERRED FROM	CODE	DCID (228) Equation or Table			DCID (12013) Gestational Age Equations and Tables
5	>>	R-INFERRED FROM	NUM				
6	>>	HAS PROPERTIES	NUM	DCID (226) Population Statistical Descriptors			
7	>	CONTAINS	NUM	(DCM, 125012, "Growth Percentile Rank")			
8	>>	INFERRED FROM	CODE	DCID (228) Equation or Table			

A.22. TID (5009) Fetal Biophysical Profile Section

	NL	Relation with Parent	Value Type	Concept Name	Used in Modality	Condition	Value Set Constraint
1			CONTAINER	DT (125006,			

2	>	HAS OBS CONTEXT	INCLUDE	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	NUM	EV (11631-9, LN,			

15	>>	HAS PROPERTIES	TEXT	(121106, DCM,			

A.23. TID (5010) Amniotic Sac Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (121070, DCM,			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3,			DT (T-F1300,
3	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = DT (11627-7, LN,
4	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11624-4, LN,
5	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11626-9, LN, Second Quadrant
6	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11625-1, LN,
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (11623-6, LN, "Fourth Quadrant
8	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (M12008-01,MRUS, "Amniotic Fluid")

A.24. TID (5011) Early Gestation Section

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125009,			
2	>	HAS OBS CONTEXT	TEXT	EV (11951-1,LN,			
3	>	HAS OBS CONTEXT	NUM	EV (11878-6,LN, "Number of			
4	>	CONTAINS	INCLUDE	DTID (5008) Fetal Biometry Group			$BiometryType= Member of {DCID (12009) Early Gestation Biometry Measurements}

A.25. TID (5012) Ovaries Section

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (121070, DCM,			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3,			DT (T-87000,
3	>	CONTAINS	INCLUDE	EV (T-87000,			$Measurement = EV (T-

4	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11829-
5	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11840-
6	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11857-
7	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (12164-
8	>	CONTAINS	INCLUDE	EV (T-87000,			$GroupName = EV (T-
9	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11830-
10	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11841-
11	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11858- Ovary Heigh
12	> >	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (12165-

A.26. TID (5013) Follicles Section

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (121070, DCM,			

2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3,			DT (T-87600, SRT,
3	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT,			$Laterality
4	>	CONTAINS	NUM	EV (11879-4, LN, of follicles in left OR EV (11880-2, of follicles in Number of follicles in the ovary.			
5	>	CONTAINS	INCLUDE	DTID (5014) Follicle Measurement Group			

A.27. TID (5014) Follicle Measurement Group

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	EV (125007, DCM,			
2	>	HAS OBS CONTEXT	TEXT	EV (12510, DCM,			Unique among all groups of same laterality
3	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (G-D705, SRT,

4	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (M11793-02, MRUS,
5	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (M11793-01, LN,
6	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (M11794-01, MRUS,
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV (11793-7, LN

A.28. TID (5015) Pelvis And Uterus Section

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	DT (125011,			
2	>	CONTAINS	CONTAINER	$GroupName			$GroupName = EV (T-
3	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Width $Width = EV (11865-
4	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Length $Length = EV (11842-2,
5	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Height $Height = EV (11859-6,
6	>>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = $Volume $Volume = EV (33192-6,
7	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV(LN,11961-0,Cervix Length)

8	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = EV(LN,12145-9,Endometrium Thickness)
9	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,M12011-01,Cervix Height)
10	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,M12011-02,Cervix Width)
11	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,C12011-03,Uterus Body)
12	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,C12011-04,UT_L/CX_L)
13	>	CONTAINS	INCLUDE	DTID (300) Measurement			$Measurement = (MRUS,M12011-03,Matrix Kindney Length)

A.29. TID (5025) OB-GYN Fetus Vascular Ultrasound Measurement Group

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	$AnatomyGroup			

							DCID (3627) Measurement Type

A.30. TID (5026) OB-GYN Pelvic Vascular Ultrasound Measurement Group

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	$AnatomyGroup			
2	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT,			DCID (244) Laterality
3	>	HAS CONCEPT MOD	TEXT	(112050, DCM, Identifier			
4	>	CONTAINS	INCLUDE	DTID (300) Measurement	√		$MeasType = DCID (12119) Vascular Ultrasound Property $Derivation = DCID (3627) Measurement Type

A.31. CID (228) Equation or Table

CSD	CV	Code Meaning
DCM	121420	Equation
DCM	121421	Equation Citation
DCM	121424	Table of Values
DCM	121422	Table of Values Citation
DCM	121423	Method Citation

A.32. CID (244) Laterality

CSD	CV	Code Meaning
SRT	G-A100	Right
SRT	G-A101	Left
SRT	G-A102	Right and left
SRT	G-A103	Unilateral

A.33. CID (3627) Measurement Type

CSD	CV	Code Meaning
SRT	R-002E1	Best value
SRT	R-00317	Mean
SRT	R-00319	Median
SRT	R-0032E	Mode
SRT	R-00355	Point source measurement
SRT	R-00353	Peak to peak
SRT	R-41D27	Visual estimation
SRT	R-10260	Estimated
SRT	R-41D2D	Calculated

CSD	CV	Code Meaning
MRUS	M12011-01	Placental Thickness
MRUS	M12005-03	Heart Area

A.35. CID (12006) Fetal Long Bones Measurements

CSD	CV	Code Meaning
LN	11966-9	Humerus length
LN	11967-7	Radius length
LN	11969-3	Ulna length
LN	11968-5	Tibia length
LN	11964-4	Fibula length
LN	11962-8	Clavicle length
LN	11963-6	Femur Length

A.36. CID (12007) Fetal Cranium

CSD	CV	Code Meaning
LN	12171-5	Lateral Ventrical width
LN	11860-4	Cisterna Magna length
LN	12146-7	Nuchal Fold thickness
LN	33070-4	Inner Orbital Diameter
LN	11629-3	Outer Orbital Diameter
LN	11863-8	Trans Cerebellar Diameter
LN	33069-6	Nuchal Translucency
LN	12170-7	Width of Hemisphere
MRUS	M12007-01	Ear Length
MRUS	M12007-02	Middle Phalanx Length
MRUS	M12007-03	Orbit
MRUS	M12007-04	OFDHC
MRUS	C12007-01	HCc

A.37. CID (12009) Early Gestation Biometry Measurements

CSD	CV	Code Meaning
LN	11957-8	Crown Rump Length
LN	11850-5	Gestational Sac Diameter
LN	33071-2	Spine Length
LN	11816-6	Yolk Sac length
LN	33069-6	Nuchal Translucency
MRUS	C12009-01	Mean Gestational Sac Diameter
MRUS	M12009-01	Gestational Sac Diameter1
MRUS	M12009-02	Gestational Sac Diameter2
MRUS	M12009-03	Gestational Sac Diameter3

A.38. CID (12013) Gestational Age Equations and Tables

CSD	CV	Code Meaning
LN	11885-1	Gestational Age by LMP
LN	11892-7	AC, Hadlock 1984
LN	11893-5	AC, Jeanty 1984
LN	33148-8	AC by GA, Merz 1988
LN	11902-4	BPD, Hadlock 1984
LN	11903-2	BPD, Hansmann 1985
LN	11905-7	BPD, Jeanty 1984
LN	33082-9	BPD, Osaka 1989
LN	33083-7	BPD, Rempen 1991
LN	11906-5	BPD, Kurtz 1980
LN	33088-6	Clavical length,Yarkoni 1985
LN	11910-7	CRL, Hadlock 1992
LN	11911-5	CRL, Hansmann 1985
LN	11917-2	CRL, Jeanty 1984
LN	11913-1	CRL, Nelson 1981
LN	33094-4	CRL, Rempen 1991
LN	11914-9	CRL, Robinson 1975
LN	33138-9	Fetal Trunk Cross-Sectional Area, Osaka 1989
LN	11920-6	FL, Hadlock 1984
LN	11922-2	FL, Hohler 1982

CSD	CV	Code Meaning
LN	11923-0	FL, Jeanty 1984
LN	11929-7	GS, Rempen 1991
LN	11932-1	HC, Hadlock 1984
LN	33112-4	HC, Hansmann 1985
LN	11934-7	HC, Jeanty 1984
LN	33111-6	HC derived, Chitty 1997
LN	11936-2	Humerus, Jeanty 1984
LN	33544-8	OFD, Hansmann 1985
LN	33134-8	TCD, Hill 1990
MRUS	F12013-01	AC, ASUM 2001
MRUS	F12013-02	AC,Nicolaides 1994
MRUS	F12013-03	BPD, ASUM 2001
MRUS	F12013-04	BPD, Merz 1991
MRUS	F12013-05	BPD, Tokyo 1989
MRUS	F12013-06	BPD-oo, Chitty 1994
MRUS	F12013-07	CRL, ASUM 2001
MRUS	F12013-08	CRL, Tokyo 1989
MRUS	F12013-24	EFW, Tokyo 1989
MRUS	F12013-09	FL, ASUM 2001
MRUS	F12013-10	FL, Chitty 1997
MRUS	F12013-12	FL, Merz 1991
MRUS	F12013-13	FL, Tokyo 1989
MRUS	F12013-14	FL,Warda,1985
MRUS	F12013-15	GS, Tokyo 1986
MRUS	F12013-17	HC derived, Chitty 1994
MRUS	F12013-16	HC, ASUM 2001
MRUS	F12013-18	HC,Nicolaides 1994
MRUS	F12013-19	Humerus Length, ASUM 2001
MRUS	F12013-20	OFD, ASUM 2001
MRUS	F12013-21	OFD,Nicolaides 1994
MRUS	F12013-22	OOD, Jeanty 1984
MRUS	F12013-23	TCD,Nicolaides 1994
MRUS	F12013-24	THD,Hansmann 1985
MRUS	F12013-25	GS, Hansmann 1985
MRUS	F12013-26	FL, Hansmann 1995

CSD	CV	Code Meaning
MRUS	F12013-43	EFW, Hadlock 1991
MRUS	F12013-44	Mean Sac Diameter Daya 1991
MRUS	F12013-45	GS,China 1997
MRUS	F12013-46	CRL,China 1997
MRUS	F12013-47	BPD,China 1997
MRUS	F12013-48	BPD,Nicolaides 1994
MRUS	F12013-49	FL,China 1997
MRUS	F12013-50	FL,Nicolaides 1994
MRUS	F12013-52	AC, Hansmann1986
MRUS	F12013-53	AC CFEF Crequat2000
MRUS	F12013-54	AC,Chitty plotted 1994
MRUS	F12013-55	CRL Robinson hp BMUS 1975
MRUS	F12015-22	FL,Osaka 1989
LN	11944-6	Ulna91 556.71</MCID 62>> BDC 170.95 536.5

CSD	CV	Code Meaning
LN	11746-5	EFW by AC, FL, HC, Hadlock 1985
LN	11884-4	Average Ultrasound Age
MRUS	F12013-27	CUA by BPD, Hadlock 1984
MRUS	F12013-28	CUA by AC, Hadlock 1984
MRUS	F12013-29	CUA by HC, Hadlock 1984
MRUS	F12013-30	CUA by FL, Hadlock 1984
MRUS	F12013-31	CUA by BPD, HC, Hadlock 1984
MRUS	F12013-32	CUA by BPD, AC, Hadlock 1984
MRUS	F12013-33	CUA by BPD, FL, Hadlock 1984
MRUS	F12013-34	CUA by HC, AC, Hadlock 1984
MRUS	F12013-35	CUA by HC, FL, Hadlock 1984
MRUS	F12013-36	CUA by AC, FL, Hadlock 1984
MRUS	F12013-37	CUA by BPD, HC, AC, Hadlock 1984
MRUS	F12013-38	CUA by BPD, HC, FL, Hadlock 1984
MRUS	F12013-39	CUA by BPD, AC, FL, Hadlock 1984
MRUS	F12013-40	CUA by HC, AC, FL, Hadlock 1984
MRUS	F12013-41	CUA by BPD, HC, AC, FL, Hadlock 1984
MRUS	F12014-01	EFW by AC,BPD,Merz 1991
MRUS	F12014-02	EFW by AC,Merz 1991
MRUS	F12014-03	EFW by BPD, TTD, Hansmann 1995
MRUS	F12014-04	EFW by BPD, FTA, FL, Osaka 1983
MRUS	F12014-05	MRUS,EFW by AC,HC,FL,Schild 2004
MRUS	F12014-06	EFW by BPD,FL,MAD,Persson 1996
LN	11738-2	EFW by AC, BPD,Hadlock 1984

A.40. CID (12015) Fetal Growth Equations and Tables

CSD	CV	Code Meaning
LN	33146-2	AC by GA, Hadlock 1984

LN

CSD	CV	Code Meaning
LN	33167-8	FL by GA, Chitty 1994
LN	33171-0	GS by GA, Rempen 1991
LN	33173-6	HC by GA, Hadlock 1984
LN	33174-4	HC derived by GA, Chitty 1994
LN	33181-9	TCD by GA Goldstein 1987
LN	33097-7	Fibula, Jeanty 1983
LN	33126-4	Radius, Jeanty 1983
MRUS	F12015-01	AC by GA, ASUM 2001
MRUS	F12015-02	AC by GA, Merz 1991
MRUS	F12015-03	AC, Jeanty 1984
MRUS	F12015-04	APAD,Merz 1991
MRUS	F12015-05	BPD by GA, ASUM 2001
MRUS	F12015-06	BPD, Hansmann 1985
MRUS	F12015-07	BPD by GA, Merz 1988
MRUS	F12015-08	BPD,Kurtz,1980
MRUS	F12015-09	BPD,Sabbagha 1978
MRUS	F12015-10	BPD, Tokyo 1989
MRUS	F12015-12	Clavical length,Yarkoni 1985
MRUS	F12015-13	CRL by GA ASUM 2001
MRUS	F12015-14	CRL, Hansmann 1985
MRUS	F12015-15	CRL, Robinson 1975
MRUS	F12015-16	CRL, Tokyo 1989
MRUS	F12015-17	EFW by GA, Hadlock 1984
MRUS	F12015-18	FL by GA, ASUM 2001
MRUS	F12015-19	FL, Hansmann 1995
MRUS	F12015-20	FL by GA, Merz 1991
MRUS	F12015-21	FL, O'Brien,1981
MRUS	F12015-22	FL, Osaka 1989
MRUS	F12015-23	FL, Tokyo, 1989
MRUS	F12015-24	FL,Warda,1985
MRUS	F12015-25	FIB,Merz,1991
MRUS	F12015-26	FTA, Osaka 1989
MRUS	F12015-27	HC by GA, ASUM 2001
MRUS	F12015-28	HC, Hansmann 1985
MRUS	F12015-29	HC by GA, Merz 1991

CSD	CV	Code Meaning
MRUS	F12015-30	Humerus Length by GA, ASUM 2001
MRUS	F12015-31	OFD by GA, ASUM 2001
MRUS	F12015-32	OFD, Hansmann 1985
MRUS	F12015-33	OFD,Merz 1991
MRUS	F12015-34	OFD,Nicolaides 1994
MRUS	F12015-35	RAD,Merz 1991
MRUS	F12015-36	TAD,Merz 1991
MRUS	F12015-37	TCD,Hill 1990
MRUS	F12015-38	THD, Hansmann 1985
MRUS	F12015-39	Tibia,Merz 1991
MRUS	F12015-40	Ulna,Merz 1991
MRUS	F12015-41	EFW by GA, Hansmann 1995
MRUS	F12015-42	FL, Jeanty 1984
MRUS	F12015-43	HC, Jeanty 1984
MRUS	F12015-44	OFD, Jeanty 1984
MRUS	F12015-45	HUM, Jeanty 1984
MRUS	F12015-46	ULNA, Jeanty 1984
MRUS	F12015-47	TIBIA, Jeanty 1984
MRUS	F12015-48	BPD, CFEF Crequat 2000
MRUS	F12015-49	HC, CFEF Crequat 2000
MRUS	F12015-50	FL, CFEF Crequat 2000
MRUS	F12015-51	TAD, CFEF Crequat 2000
MRUS	F12015-52	OOD, Jeanty 1984
MRUS	F12015-53	AC, CFEF Crequat 2000
MRUS	F12015-58	DV PIV,Baschat 2003
MRUS	F12015-59	DV PLI,Baschat 2003
MRUS	F12015-60	DV PVIV,Baschat 2003
MRUS	F12015-61	DV S/a,Baschat 2003
LN	33182-7	HC/AC by GA, Campbell 1977

A.41. CID (12119) Vascular Ultrasound Property

CSD	CV	Code Meaning
INCLUDE CID 12120 Blood Velocity Measurements		
INCLUDE CID 12121 Vascular Indices and Ratios		

CSD	CV	Code Meaning
INCLUDE CID 12122 Other Vascular Properties		

A.42. CID (12120) Blood Velocity Measurements

CSD	CV	Code Meaning
LN	11653-3	End Diastolic Velocity
LN	11665-7	Minimum Diastolic Velocity
LN	11726-7	Peak Systolic Velocity
LN	11726-7	Peak Velocity
LN	20352-1	Time averaged mean velocity
LN	11692-1	Time averaged peak velocity

A.43. CID (12121) Vascular Indices and Ratios

CSD	CV	Code Meaning
LN	12008-9	Pulsatility Index
LN	12023-8	Resistivity Inde6.5 479(s)25(i)-24(s)25(t)-24(i)

MRUS	M12119-06	Vol Flow(TAMAX)
MRUS	M12119-07	Vol Flow(TAMEAN)

A.45. CID (12140) Pelvic Vasculature Anatomical Location

CSD	CV	Code Meaning
SRT	T-46980	Ovarian Artery
SRT	T-46820	Uterine Artery

A.46. CID (12141) Fetal Vasculature Anatomical Location

CSD	CV	Code Meaning
SRT	T-42000	Aorta
SRT	T-D0765	Descending Aorta
SRT	T-45600	Middle Cerebral Artery
MRUS	V12141-01	Ductus Venosus
SRT	T-F1810	Umbilical Artery
SRT	T-F1820	Umbilical Vein
SRT	T-F1412	Vitelline Artery of Placenta

A.47. CID (SELFCID-1) Fetal Z-Score

CSD	CV	Code Meaning
LN	18015-8	Aortic Root Diameter
LN	18020-8	Main Pulmonary Artery Diameter
LN	18154-5	Interventricular Septum Diastolic Thickness
LN	18158-6	Interventricular Septum Systolic Thickness
MRUS	M18015-8	Aortic Root Diameter(Z Score)
MRUS	M18020-8	Main Pulmonary Artery Diameter(Z Score)
MRUS	C12201-06	Left Ventricular Diameter/Right Ventricular Diameter
MRUS	C12201-07	Left Ventricular Diameter/Right Ventricular Diameter(Z Score)
MRUS	C12205-03	Left Atrium Diameter / Right Atrium Diameter
MRUS	C12205-04	Left Atrium Diameter / Aorta Diameter
MRUS	C12205-05	Left Atrium Diameter / Aorta Diameter(Z Score)
MRUS	C12212-01	Aorta Diameter/Main Pulmonary Artery Diameter
MRUS	C12212-03	Aorta Diameter/Main Pulmonary Artery Diameter(Z Score)
MRUS	M12201-01	Left ventricular short-axis diameter at end diastole
MRUS	M12201-08	Left ventricular short-axis diameter at end diastole(Z Score)

MRUS	M12201-02	Left ventricular short-axis diameter at end systole
MRUS	M12201-03	Left ventricular Diameter
MRUS	M12201-09	Left ventricular Diameter(Z Score)
MRUS	M12201-04	interventricular septal thichness
MRUS	M12201-05	Left Ventricular Outflow Tract Diameter
MRUS	M12204-01	Right ventricular short-axis diameter at end diastole
MRUS	M12204-07	Right ventricular short-axis diameter at end diastole(Z Score)
MRUS	M12204-02	Right ventricular short-axis diameter at end systole
MRUS	M12204-03	Right ventricular Diameter
MRUS	M12204-08	Right ventricular Diameter(Z Score)
MRUS	M12204-09	Right ventricular area(Z Score)
MRUS	M12204-04	Right ventricular area
MRUS	M12206-01	Right Atrium Diameter
MRUS	M12204-05	Right Ventricular Outflow Tract Diameter
MRUS	M12205-01	

MODALITY Label	***DICOM Mapping***
CIHC	C12004-04, MRUS,Cephalic Index by HC
MAD	C12005-06,MRUS,Mean Abdominal Diameter
AC	11979-2,LN,Abdominal Circumference
BPD	11820-8,LN,Biparietal Diameter
FL	11963-6,LN,Femur Length
HC	11984-2,LN,Head Circumference
OFD	11851-3,LN,Occipital-Frontal Diameter
APAD	11818-2,LN,Anterior-Posterior Abdominal Diameter
TC	11988-3,LN,Thoracic Circumference
TAD	11862-0,LN,Tranverse Abdominal Diameter
TTD	11864-6,LN,Transverse Thoracic Diameter
APTD	11819-0,LN,Anterior-Posterior Trunk Diameter
FTA	33068-8,LN,Thoracic Area
TCD	11863-8,LN,Trans Cerebellar Diameter
Foot	11965-1,LN,Foot length
Cist Magna	11860-4,LN,Cisterna Magna
AXT	33191-8,LN,APAD * TAD
F-kidney	M12005-05, MRUS, Fetal Kidney length
THD	M12005-01,MRUS,Thoracic Diameter
HrtC	M12005-02,MRUS,Heart Circumference
HUM	11966-9,LN,Humerus length
RAD	11967-7,LN,Radius length
Ulna	11969-3,LN,Ulna length
Tibia	11968-5,LN,Tibia length
FIB	11964-4,LN,Fibula length
CLAV	11962-8,LN,Clavicle length
LVW	12171-5,LN,Lateral Ventrical width
NF	12146-7,LN,Nuchal Fold thickness
IOD	33070-4,LN,Inner Orbital Diameter
OOD	11629-3,LN,Outer Orbital Diameter
TCD	11863-8,LN,Trans Cerebellar Diameter
NT	33069-6,LN,Nuchal Translucency
HW	12170-7,LN,Width of Hemisphere
Ear	M12007-01,MRUS,Ear Length

MODALITY Label	***DICOM Mapping***
MP	M12007-02,MRUS,Middle Phalanx Length
Orbit	M12007-03,MRUS,Orbit
OFD(HC)	M12007-04,MRUS,OFDHC
HC(c)	C12007-01,MRUS,HCc
AF1	11624-4,LN,First Quadrant Diameter
AF2	11626-9,LN,Second Quadrant Diameter
AF3	11625-1,LN,Third Quadrant Diameter
AF4	11623-6,LN,Fourth Quadrant Diameter
AF	M12008-01,MRUS,Amniotic Fluid
CRL	11957-8,LN,Crown Rump Length
GS	11850-5,LN,Gestational Sac Diameter
Vertebrae	33071-2,LN,Spine Length
YS	11816-6,LN,Yolk Sac length
NT	33069-6,LN,Nuchal Translucency
Mean Sac Diam	C12009-01,MRUS,Mean Gestational Sac Diameter
Cervix L	11961-0,LN,Cervix Length
Cervix L	11961-0,LN,Cervix Length
Endo	12145-9,LN,Endometrium Thickness
Cervix H	M12011-01,MRUS,Cervix Height
Cervix W	M12011-02,MRUS,Cervix Width
Uterus Body	C12011-03,MRUS,Uterus Body
UT-L/CX-L	C12011-04,MRUS,UT_L/CX_L
Mat Kidney	M12011-03,MRUS,Matrix Kindney Length
AFI	11627-7,LN,Amniotic Fluid Index
Ovary W	11829-9, LN, Left Ovary Width;11830-7, LN, Right Ovary Width
Ovary L	11840-6, LN, Left Ovary Length;11841-4, LN, Right Ovary Length
Ovary H	11857-0, LN, Left Ovary Height;11858-8, LN, Right Ovary Height
Ovary Vol	12164-0, LN, Left Ovary Volume;12165-7, LN, Right Ovary Volume
Follicle1 L	M11793-02, MRUS, Follicle Length
Follicle2 L	M11793-02, MRUS, Follicle Length
Follicle3 L	M11793-02, MRUS, Follicle Length
Follicle4 L	M11793-02, MRUS, Follicle Length
Follicle5 L	M11793-02, MRUS, Follicle Length
Follicle6 L	M11793-02, MRUS, Follicle Length

MODALITY Label	*DICOM Mapping*
Follicle7 L	M11793-02, MRUS, Follicle Length
Follicle8 L	M11793-02, MRUS, Follicle Length
Follicle9 L	M11793-02, MRUS, Follicle Length
Follicle10 L	M11793-02, MRUS, Follicle Length
Follicle11 L	M11793-02, MRUS, Follicle Length
Follicle12 L	M11793-02, MRUS, Follicle Length
Follicle13 L	M11793-02, MRUS, Follicle Length
Follicle14 L	M11793-02, MRUS, Follicle Length
Follicle15 L	M11793-02, MRUS, Follicle Length
Follicle16 L	M11793-02, MRUS, Follicle Length
UT W	11865-3,LN,Uterus Width
UT L	11842-2,LN,Uterus Length
UT H	11859-6,LN,Uterus Height
UT Vol	33192-6,LN,Uterus Volume
Follicle1 W	M11793-01,MRUS,Follicle Width
Follicle2 W	M11793-01,MRUS,Follicle Width
Follicle3 W	M11793-01,MRUS,Follicle Width
Follicle4 W	M11793-01,MRUS,Follicle Width
Follicle5 W	M11793-01,MRUS,Follicle Width
Follicle6 W	M11793-01,MRUS,Follicle Width
Follicle7 W	M11793-01,MRUS,Follicle Width
Follicle8 W	M11793-01,MRUS,Follicle Width
Follicle9 W	M11793-01,MRUS,Follicle Width
Follicle10 W	M11793-01,MRUS,Follicle Width
Follicle11 W	M11793-01,MRUS,Follicle Width
Follicle12 W	M11793-01,MRUS,Follicle Width
Follicle13 W	M11793-01,MRUS,Follicle Width
Follicle14 W	M11793-01,MRUS,Follicle Width
Follicle15 W	M11793-01,MRUS,Follicle Width
Follicle16 W	M11793-01,MRUS,Follicle Width
Follicle1 Vol	G-D705,SRT,Volume
Follicle2 Vol	G-D705,SRT,Volume
Follicle3 Vol	G-D705,SRT,Volume
Follicle4 Vol	G-D705,SRT,Volume

MODALITY Label	*DICOM Mapping*
EFW(Campbell)	11727-5,LN,Estimated Weight
EFW(Hadlock1)	11727-5,LN,Estimated Weight
EFW(Hadlock2)	11727-5,LN,Estimated Weight
EFW(Hadlock3)	11727-5,LN,Estimated Weight
EFW(Hadlock4)	11727-5,LN,Estimated Weight
EFW(Hansmann)	11727-5,LN,Estimated Weight
EFW(Merz1)	11727-5,LN,Estimated Weight
EFW(Merz2)	11727-5,LN,Estimated Weight
EFW(Osaka)	11727-5,LN,Estimated Weight
EFW(Shepard)	11727-5,LN,Estimated Weight
EFW(Tokyo)	11727-5,LN,Estimated Weight
PL Thickness	M12011-01,MRUS,Placental Thickness
HrtA	M12005-03,MRUS,Heart Area
Facial angle	M12005-04,MRUS,Facial angle
Sac Diam1	M12009-01,MRUS,Gestational Sac Diameter1
Sac Diam2	M12009-02,MRUS,Gestational Sac Diameter2
Sac Diam3	M12009-03,MRUS,Gestational Sac Diameter3

A.48.2. Vasculature Anatomic Location

MODALITY Vasculature Anatomic Location	*DICOM Mapping*
Ovarian A	T-46980, SRT, Ovarian Artery
Ut A	T-46820, SRT, Uterine Artery
Fetal Ao	T-42000, SRT, Aorta
Desc Aorta	T-D0765, SRT, Descending Aorta
Duct Veno	V12141-01, MRUS, Ductus Veno
Umb A	T-F1810, SRT, Umbilical Artery
Umb V	T-F1820, SRT, Umbilical Vein
Placenta A	T-F1412, SRT, Vitelline Artery of Placenta

A.48.3. OB-GYN Vascular Measurements

MODALITY Label	*DICOM Mapping*
<Vasculature Anatomic Location> ED	11653-3, LN, End Diastolic Velocity
<Vasculature Anatomic Location> MD	11665-7 , LN, Minimum Diastolic Velocity
<Vasculature Anatomic Location> PS	11726-7, LN, Peak Systolic Velocity

MODALITY Label	*DICOM Mapping*
<Vasculature Anatomic Location> TAMEAN	20352-1, LN, Time averaged mean velocity
<Vasculature Anatomic Location> TAMAX	11692-1, LN, Time averaged peak velocity
<Vasculature Anatomic Location> PV	11726-7, LN, Peak Velocity
<Vasculature Anatomic Location> PI	12008-9, LN, Pulsatility Index
<Vasculature Anatomic Location> RI	12023-8, LN, Resistivity Index
<Vasculature Anatomic Location> S/D	12144-2, LN, Systolic to Diastolic Velocity Ratio
<Vasculature Anatomic Location> D/S	M12119-04, MRUS, Diastolic to SystolicVelocity Ratio
<Vasculature Anatomic Location> AT	20168-1, LN, Acceleration Time
<Vasculature Anatomic Location> DT	20217-6, LN, Deceleration Time
<Vasculature Anatomic Location> PPG	20247-3, LN, Peak Gradient
<Vasculature Anatomic Location> MPG	20256-4, LN, Mean Gradient
<Vasculature Anatomic Location> MMPG	M12119-01, MRUS, Mean Velocity Mean Pressure Gradient
<Vasculature Anatomic Location> VTI	M12119-02, MRUS,Velocity-Time Integral

IVS	M12201-04,MRUS,interventricular septal thichness
LVOT Diam	M12201-05,MRUS,Left Ventricular Outflow Tract Diameter
RVIDd	M12204-01,MRUS,Right ventricular short-axis diameter at end diastole
<Z.Scores> RVIDd	M12204-07,MRUS,Right ventricular short-axis diameter at end diastole(Z Score)
RVIDs	M12204-02,MRUS,Right ventricular short-axis diameter at end systole
RV Diam	M12204-03,MRUS,Right ventricular Diameter
<Z.Scores> RV Diam	M12204-08,MRUS,Right ventricular Diameter(Z Score)
RA Diam	M12206-01,MRUS,Right Atrium Diameter
RV Area	M12204-04,MRUS,Right ventricular area
<Z.Scores> RV Area	M12204-09,MRUS,Right ventricular area(Z Score)
RVOT Diam	M12204-05,MRUS,Right Ventricular Outflow Tract Diameter
LA Diam	M12205-01,MRUS,Left Atrium Diameter
LA Area	M12205-02,MRUS,Left Atrium area
RA Area	M12206-02,MRUS,Right Atrium area
LV Area	M12240-01,MRUS,Left ventricular area
<Z.Scores> LV Area	M12240-02,MRUS,Left ventricular area(Z Score)

ZScoreFL

Upper Extremities	FG4031-05,MRUS,Upper Extremities
Lower Extremities	FG4031-06,MRUS,Lower Extremities
Cardiac Activity	FG12239-01,MRUS,Cardiac Activity
4C HEART	FG4031-08,MRUS,4C HEART
Aorta	T-42000,SNM3,Aorta
Pulmonary Artery	T-44000,SNM3,Pulmonary Artery
ARCH	FG3010-01,MRUS,ARCH
Lateral Ventricles	FG4030-02,MRUS,Lateral Ventricles
Cisterna Magna	11860-4,LN,Cisterna Magna
Cerebellum	T-A600A,SNM3,Cerebellum
CSP	FG4030-03,MRUS,CSP
Cervical Spine	T-11501,SNM3,Cervical Spine
Thoracic Spine	T-11502,SNM3,Thoracic Spine
Lumbar Spine	T-11503,SNM3,Lumbar Spine
Sacral Spine	FG4031-,MRUS,Sacral Spine
Placental Location	FG12011-01,MRUS,Placental Location
Amniotic Fluid	FG12011-02,MRUS,Amniotic Fluid
Placental Grade	FG12011-03,MRUS,Placental Grade
Adnexa	FG12011-03,MRUS,Adnexa
Ovaries	T-87000,SRT,Ovary
Kidney	T-71000,SRT,Kidney
Cervix	T-83200,SRT,Cervix

B. Appendix : Cardiac structured reporting template

This appendix lists the DICOM Structured Report (SR) mappings used in the

Cardiac Structured Reports of ultrasound system SR files.

The mappings are organized in a manner similar to the DICOM SR Templates as described in PS 3.16 of the DICOM Standard. The Cardiac Report mappings follow the DICOM SR Template TID 5200: Cardiac Ultrasound Procedure Report, except where noted.

All private code values use the Coding Scheme Designator "MRUS".

B.1. TID (5200) Echocardiography Procedure Report

This template forms the top of a content tree that allows an ultrasound system to describe the results of an adult echocardiography imaging procedure.

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1			CONTAINER	EV (125200, DCM,			
2	>	HAS CONCEPT MOD	INCLUDE	DTID (1204) Language of Content Item and Descendants			
3	>	HAS OBS CONTEXT	INCLUDE	DTID (1001) Observation Context			
4	>	CONTAINS	INCLUDE	DTID (5201) Echocardiography Patient Characteristics			
5	>	CONTAINS	CONTAINER				
6	>>	CONTAINS	IMAGE	No purpose of reference			
7	>	CONTAINS	INCLUDE	DTID(SELFTEM-2)Echo Procedure Summary Section			
8	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			

							(12200) Echocardiography Left Ventricle
9	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-V $MeasType = DCID (12204) Echocardiography Right Ventricle
10	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T- $MeasType = DCID (12205) Echocardiography Left Atrium
11	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T- $MeasType = DCID (12206) Echocardiography Right Atrium

12

							Echocardiography Pulmonic Valve
15	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-35100, SRT, $MeasType = DCID (12208) Echocardiography Tricuspid Valve
16	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-42000, SRT, $MeasType= DCID (12212) Echocardiography Aorta
17	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-44000, SRT, $MeasType DCID (12210) = Echocardiography Pulmonary Artery
18	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T- $MeasType = DCID (12215) Echocardiography Vena Cavae
19	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (T-48581, SRT, $MeasType = DCID (12214) Echocardiography Pulmonary Veins
20	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (P5-30031, SRT, DCID (12217)

							Echocardiography Cardiac Shunt
21	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (D4-30000, SRT, of Cardiovascular = DCID (12218) Echocardiography Congenital
22	>	CONTAINS	INCLUDE	DTID (5204) Wall Motion Analysis			
23	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (D3-90000, SRT, $MeasType = DCID (90000) Pericardial disease
24	>	CONTAINS	INCLUDE	DTID (5202) Echo Section			$SectionSubject = EV (G- $MeasType = DCID (12220) Echocardiography Common Measurements

B.2. TID(1001) Observation Context

This template specifies attributes of observation context that may be defined, extended or replaced at any location in the SR tree.

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Condition	Value Set Constraint
1	>	HAS OBS CONTEXT	CODE	EV (121005,DCM,			(121006,DCM,
2	>	HAS OBS CONTEXT	PNAME	EV (121008,DCM,			Operator from Info

3	>	HAS OBS CONTEXT	TEXT	EV (121009,DCM,			Institution Name (0008,0080) of the General Equipment Module
4	>	HAS OBS CONTEXT	CODE	EV (121010,DCM, Role in the			(121093, DCM, "Sonographer")
5	>	HAS OBS CONTEXT	CODE	EV (121024, DCM,			(121025, DCM, "Pati
6	>	HAS OBS CONTEXT	PNAME	EV (121029,DCM,			(0010,0010) in Patient Module
7	>	HAS OBS CONTEXT	DATE	EV (121031,DCM,			Date (0010,0030) in Patient Module
8	>	HAS OBS CONTEXT	CODE	EV (121032,DCM,			value equivalent to (0010,0040) in Patient Module
9	>	HAS OBS CONTEXT	NUM	EV (121033,DCM,			(0010,1010) in Patient Study Module

B.3. TID (5201) Echocardiography Patient Characteristics

	NL	Rel with Parent	VT	Concept Name	Used in Modality	Value Set Constraint	Comments
1			CONTAINER	EV (121118, DCM,			
2	>	CONTAINS	NUM	EV (121033, DCM,		Units = DCID (7456) Units of Measure for Age	from Info
3	>	CONTAINS	CODE	EV (121032, DCM,		DCID (7455) Sex	from worklist or Info
4	>	CONTAINS	NUM	EV (8867-			from Info
5	>	CONTAINS	NUM	EV (F-008EC, SRT,			from Info

6	>	CONTAINS	NUM	EV (F-008ED, SRT, "Diastolic Blood Pressure")			from Info
7	>	CONTAINS	NUM	EV(18070-3,LN,"Right Atrium Systolic Pressure")			from Info
8	>	CONTAINS	NUM	EV (8302-			from worklist or Info
9	>	CONTAINS	NUM	EV (29463-			from worklist or Info
10	>	CONTAINS	NUM	EV (8277-			from Info
11	>>	INFERRED FROM	CODE	EV (8278-4, LN, "Body Surface Area Formula")		BCID (3663) Body Surface Area Equations	

B.4. TID (SELFTMP-2) Echo Procedure Summary Section

This is a private template referenced by TID(5200).

	NL	Rel with Parent	VT	Concept Name	Used in Modality	Value Set Constraint	Comment
1			CONTAINER	DT(12111,DCM,"Summary")			
2	>	CONTAINS	TEXT	EV(121106,DCM,"Comment")			from Info
3	>	CONTAINS	TEXT	(I12101-01,MRUS,"Primary Indications")			from Info
4	>	CONTAINS	TEXT	(I12101-02,MRUS,"Secondary Indications")			from Info
5	>	CONTAINS	TEXT	(I12101-03,MRUS,"CPT4 Code")			from Info
6	>	CONTAINS	TEXT	(I12101-04,MRUS,"CPT4 Description")			from Info
	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")			from report interface Comment
8	>	CONTAINS	TEXT	(I12101-05,MRUS,"Prompt")			from report interface Comment
9	>	CONTAINS	TEXT	(121071,DCM,"Findings")			from report interface

							Comment

B.5. TID (5202) ECHO SECTION

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1			CONTAINER	EV (121070,			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT,		$SectionSubject = EV (T-32600,	
3	>	CONTAINS	CONTAINER	DT (125007, DCM,			
4	>>	HAS CONCEPT MOD	CODE	EV (G-		BCID (12224) Ultrasound Image Modes	
5	>>	HAS CONCEPT MOD	CODE	DT			
6	>>	CONTAINS	INCLUDE	DTID (5203) Echo Measurement		$Measurement= $MeasType = DCID (12200) Echocardiography Left Ventricle $Method=CID (12227) Echocardiography Measurement Method	

B.6. TID (5203) Echo Measurement

	NL	Relation with Parent	Value Type	Concept Name	Used in MODALITY	Value Set Constraint	Comment

1			INCLUDE	DTID (300) Measurement		$Measurement = $Measurement $Method = $Method $TargetSite = BCID (12236) Echo Anatomic Sites $TargetSiteMod = BCID (12237) Echocardiography Anatomic Site Modifiers	
2	>	HAS CONCEPT MOD	CODE	EV(G-C036,SRT,"Measurement Method")		This row is used only if the measurement or calculation this template is invoked with mandates it. Otherwise this row is not used. The values are taken from the BCID 12227	
3	>	HAS CONCEPT MOD	CODE	EV (G-		BCID (12221) Flow Direction	
4	>	HAS CONCEPT MOD	CODE	EV (R-		DCID (12234) Respiration State	
5	>	HAS CONCEPT MOD	CODE	EV (R-		DCID (12233) Respiration State	
6	>	HAS ACQ CONTEXT	CODE	EV (G-		DCID (12224) Ultrasound Image Modes	
7	>	HAS ACQ CONTEXT	CODE			BCID (12226) Echocardiography Image View	

B.7. CID (12200) Echocardiography Left Ventricle

INCLUDE CID 12220 Echocardiography Common Measurements
INCLUDE CID 12201 Left Ventricle Linear
INCLUDE CID 12240 Left Ventricle Area
INCLUDE CID 12202 Left Ventricle Volume
INCLUDE CID 12222 Orifice Flow Properties
INCLUDE CID 12203 Left Ventricle Other
INCLUDE CID 12239 Cardiac Output Properties

B.8. CID (12201) Left Ventricle Linear

CSD	CV	Code Meaning
LN	29436-3	Left Ventricle Internal End Diastolic Dimension
LN	29438-9	Left Ventricle Internal Systolic Dimension
LN	18051-3	Left Ventricular Fractional Shortening
LN	18154-5	Interventricular Septum Diastolic Thickness

1 0 0 1 161.598 514.4 cm BT /F3 7.92 Tf 12 Tz 0 g[(12 Tf1Tf1 0 0.72 0.7437.16 50.64Tf1T 18.744 reW* n /P <</64Tf1T 1

CSD	CV	Code Meaning
LN	18148-7	Left Ventricular End Systolic Volume
LN	18043-0	Left Ventricular Ejection Fraction

B.10. CID (12203) Left Ventricle Other

CSD	CV	Code Meaning
LN	18087-7	Left Ventricle Mass
LN	18071-1	Left Ventricular Isovolumic Relaxation Time
SRT	G-037E	Left Ventricular Isovolumic Contraction Time
SRT	G-037F	Left Ventricular Index of Myocardial Performance
MRUS	M12203-01	Left Ventricle Pre-Ejection Period
MRUS	M12203-02	Left Ventricle Ejection Time
MRUS	C12203-01	Left ventricular Mass Weight Index
MRUS	C12203-02	Left Ventricle Pre-Ejection Period to Ejection Time Ratio

B.11. CID (12204) Echocardiography Right Ventricle

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
INCLUDE CID 12239 Cardiac Output Properties		
LN	20304-2	Right Ventricular Internal Diastolic Dimension
LN	20305-9	Right Ventricular Internal Systolic Dimension
SRT	G-0381	Right Ventricular Index of Myocardial Performance
SRT	G-0380	Right Ventricular Peak Systolic Pressure
LN	18153-7	Right Ventricular Anterior Wall Diastolic Thickness
LN	18157-8	Right Ventricular Anterior Wall Systolic Thickness
MRUS	M12204-01	Right ventricular Major
MRUS	M12204-02	Right ventricular Minor
MRUS	M12204-03	Right ventricular Area at end-diastole
MRUS	M12204-04	Right ventricular Area at end-systole
MRUS	M12204-05	Right Ventricle Pre-Ejection Period
MRUS	M12204-06	Right Ventricle Ejection Time
MRUS	C12204-01	Right Ventricle Pre-Ejection Period to Ejection Time Ratio

B.12. CID (12205) Echocardiography Left Atrium

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	29469-4	Left Atrium Antero-posterior Systolic Dimension
LN	17985-3	Left Atrium to Aortic Root Ratio
LN	17977-0	Left Atrium Systolic Area
SRT	G-0383	Left Atrium Systolic Volume
MRUS	M12205-01	Left atrium Major
MRUS	M12205-02	Left atrium Minor
MRUS	C12205-01	Aortic Root to Left Atrium Ratio

B.13. CID (12206) Echocardiography Right Atrium

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	17988-7	Right Atrium Systolic Area
MRUS	M12206-01	Right atrium Major
MRUS	M12206-02	Right atrium Minor
MRUS	M12206-03	Right atrium Volume

B.14. CID (12207) Echocardiography Mitral Valve

CSD	CV	Code Meaning
SRT	F-32120	Stroke Volume
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
INCLUDE CID 12239 Cardiac Output Properties		
LN	17978-8	Mitral Valve A-Wave Peak Velocity
LN	18037-2	Mitral Valve E-Wave Peak Velocity
LN	18038-0	Mitral Valve E to A Ratio
SRT	G-0386	Mitral Valve AT/DT Ratio
LN	18040-6	Mitral Valve E-F Slope by M-Mode
LN	18036-4	Mitral Valve EPSS, E wave
SRT	G-0385	Mitral Valve A-Wave Duration

CSD	CV	Code Meaning
SRT	G-0387	Mitral Valve Closure to Opening Time
LN	18035-6	Mitral Regurgitation dP/dt derived from Mitral Reg. velocity
MRUS	M12207-01	Mitral valve cusp separate distance
MRUS	M12207-02	Mitral Valve D-E Slope
MRUS	M12207-03	Amplitude of the A wave
MRUS	M12207-04	Amplitude of the E wave
MRUS	M12207-05	Amplitude from D point to E point
MRUS	M12207-06	Mitral Valve E-wave Pressure Gradient
MRUS	M12207-07	Mitral Valve A-wave Pressure Gradient
MRUS	M12207-08	E wave Velocity Time Integral
MRUS	M12207-9	A wave Velocity Time Integral
MRUS	M12207-10	Mitral Valve E-Wave Duration
MRUS	M12207-11	Systolic Velocity of the Mitral Annulus(medial)
MRUS	M12207-12	Early diastolic velocity of the mitral annulus(medial)
MRUS	M12207-13	Late diastolic velocity of the mitral annulus(medial)
MRUS	M12207-14	Early diastolic velocity to Late diastolic velocity Ratio
MRUS	M12207-15	Acceleration Time of Early diastolic velocity
MRUS	M12207-16	Acceleration Rate of Early diastolic velocity
MRUS	M12207-17	Deceleration Time of Early diastolic velocity
MRUS	M12207-18	Deceleration Rate of Early diastolic velocity
MRUS	M12207-19	Systolic Velocity of the Mitral Annulus(lateral)
MRUS	M12207-20	Early diastolic velocity of the mitral annulus(lateral)
MRUS	M12207-21	Late diastolic velocity of the mitral annulus(lateral)
MRUS	M12207-22	Early diastolic velocity to Late diastolic velocity Ratio
MRUS	M12207-23	Acceleration Time of Early diastolic velocity
MRUS	M12207-24	Acceleration Rate of Early diastolic velocity
MRUS	M12207-25	Deceleration Time of Early diastolic velocity
MRUS	M12207-26	Deceleration Rate of Early diastolic velocity
MRUS	M12207-27	Mitral Stenosis Radius
MRUS	M12207-28	Mitral Stenosis Aliasing Velocity
MRUS	M12207-29	Mitral Stenosis Maximum Velocity
MRUS	M12207-30	Mitral Stenosis Area
MRUS	C12207-01	Mitral Stenosis Maximum Pressure Gradient

B.15. CID (12208) Echocardiography Tricuspid Valve

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
LN	18031-5	Tricuspid Valve E Wave Peak Velocity
LN	18030-7	Tricuspid Valve A Wave Peak Velocity
LN	18039-8	Tricuspid Valve E to A Ratio
SRT	G-0389	Tricuspid Valve Closure to Opening Time
MRUS	M12208-01	Tricuspid Valve E-Wave Duration
MRUS	M12208-02	Tricuspid Valve E Wave Pressure Gradient
MRUS	M12208-03	Tricuspid Valve A Wave Pressure Gradient
MRUS	M12207-35	MV E/Ea

B.16. CID (12209) Echocardiography Pulmonic Valve

INCLUDE CID 12220 Echocardiography Common Measurements
INCLUDE CID 12222 Orifice Flow Properties

B.17. CID (12210) Echocardiography Pulmonary Artery

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	18020-8	Main Pulmonary Artery Diameter
LN	18021-6	Right Pulmonary Artery Diameter
LN	18019-0	Left Pulmonary Artery Diameter
SRT	G-038A	Main Pulmonary Artery Peak Velocity

CSD	CV	Code Meaning
SRT	G-0382	Ratio of Aortic Valve Acceleration Time to Ejection Time

B.19. CID (12212) Echocardiography Aorta

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
LN	18015-8	Aortic Root Diameter
LN	18011-7	Aortic Arch Diameter
LN	18012-5	Ascending Aortic Diameter
LN	18014-1	Aortic Isthmus Diameter
LN	18013-3	Descending Aortic Diameter
MRUS	M12212-01	Aortic Sinotubular junction Diameter
MRUS	M12212-02	Aortic Sinus Diameter
MRUS	M12212-03	Ductus Artery Diameter
MRUS	M12212-04	Previous Ductal Diameter
MRUS	M12212-05	Left Coronary Artery Diameter
MRUS	M12212-06	Right Coronary Artery Diameter
MRUS	C12212-02	Aortic Sinotubular junction Diameter/Aorta Root Diameter

B.20. CID (12214) Echocardiography Pulmonary Veins

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
SRT	G-038B	Pulmonary Vein A-Wave Duration
SRT	G-038D	Pulmonary Vein D-Wave Velocity Time Integral/
SRT	G-038C	Pulmonary Vein S

CSD	CV	Code Meaning
LN	18006-7	Inferior Vena Cava Diameter
MRUS	M12215-01	Superior Vena Cava Diameter

B.22. CID (12217) Echocardiography Cardiac Shunt

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12239 Cardiac Output Properties		
LN	29462-9	Pulmonary-to-Systemic Shunt Flow Ratio
MRUS	M12217-01	Pulmonary-sub-Systemic Shunt Flow Difference

B.23. CID (12218) Echocardiography Congenital

CSD	CV	Code Meaning
INCLUDE CID 12220 Echocardiography Common Measurements		
INCLUDE CID 12222 Orifice Flow Properties		
MRUS	M12218-01	Patent Ductus Arteriosus Diameter
MRUS	M12218-02	Patent Foramen Ovale Diameter
MRUS	M12218-03	Patent Ductus Arteriosus Diastolic Velocity
MRUS	M12218-04	Patent Ductus Arteriosus Systolic Velocity
MRUS	M12218-05	Coarctation of Pre-Ductus Velocity
MRUS	M12218-06	Coarctation of Post-Ductus Velocity
MRUS	M12218-07	Patent Ductus Arteriosus Diastolic Peak Gradient
MRUS	M12218-08	Patent Ductus Arteriosus Systolic Peak Gradient
MRUS	M12218-09	Coarctation of Pre-Ductus Peak Gradient
MRUS	M12218-10	Coarctation of Post-Ductus Peak Gradient

B.24. CID (12220) Echocardiography Common Measurements

CSD	CV	Code Meaning
LN	8867-4	Heart rate

B.25. CID (12221) Flow Direction

CSD	CV	Code Meaning
SRT	R-42047	Antegrade Flow
SRT	R-42E61	Regurgitant Flow

B.26. CID (12222) Orifice Flow Properties

CSD	CV	Code Meaning
SRT	G-038E	Cardiovascular Orifice Area
SRT	G-038F	Cardiovascular Orifice Diameter
SRT	G-0390	Regurgitant Fraction
LN	11726-7	Peak Velocity
LN	20352-1	Mean Velocity
LN	20247-3	Peak Gradient
LN	20256-4	Mean Gradient
LN	20354-7	Velocity Time Integral
LN	20168-1	Acceleration Time
LN	11653-3	End Diastolic Velocity
LN	20280-4	Pressure Half-Time
LN	20217-6	Deceleration Time
LN	33878-0	Volume Flow
LN	34141-2	Peak Instantaneous Flow Rate
LN	20216-8	Deceleration Slope
MRUS	M12222-05	Aliasing Velocity
MRUS	M12222-04	Time
MRUS	M12222-02	Acceleration Slope
MRUS	M12222-06	Flow Radius
MRUS	M12222-01	Angle
MRUS	M12222-08	Presure Gradient at end-Diastole
MRUS	M12222-07	Acceleration Time/Deceleration Time

B.27. CID (12224) Ultrasound Image Modes

CSD	CV	Code Meaning
SRT	G-03A2	2D mode
SRT	G-0394	M mode
SRT	R-409E2	Doppler Color Flow
SRT	G-0394	M mode
SRT	R-409E4	Doppler Pulsed
SRT	R-409E3	Doppler Continuous Wave
DCM	125230	Power Doppler
DCM	125231	3D mode
MRUS	IM12224-01	Tissue Doppler Imaging

B.28. CID (12226) Echocardiography Image View

CSD	CV	Code Meaning
SRT	G-A19B	Apical two chamber
SRT	G-A19C	Apical four chamber
SRT	G-0395	Apical long axis
SRT	G-0396	Parasternal long axis
SRT	G-0397	Parasternal short axis
SRT	G-0398	Parasternal short axis at the aortic valve level
SRT	G-0399	Parasternal short axis at the level of the mitral chords
SRT	G-039A	Parasternal short axis at the Mitral Valve level
SRT	G-039B	Parasternal short axis at the Papillary Muscle level
SRT	G-039C	Right Ventricular Inflow Tract View
SRT	G-039D	Right Ventricular Outflow Tract View
SRT	G-039E	Subcostal long axis
SRT	G-039F	Subcostal short axis
SRT	G-03A0	Suprasternal long axis
SRT	G-03A1	Suprasternal short axis

B.29. CID (12227) Echocardiography Measurement Method

INCLUDE CID 12228 Echocardiography Volume Methods
INCLUDE CID 12229 Echocardiography Area Methods

INCLUDE CID 12231 Volume Flow Methods
INCLUDE CID 12232 Myocardium Mass Methods

B.30. CID (12228) Volume Methods

CSD	CV	Code Meaning
DCM	125204	Area-Length Biplane
DCM	125205	Area-Length Single Plane
DCM	125211	Biplane Ellipse
DCM	125226	Single Plane Ellipse
DCM	125206	Cube Method
DCM	125207	Method of Disks, Biplane
DCM	125208	Method of Disks, Single Plane
DCM	125209	Teichholz
MRUS	VM12228-01	Bullet
MRUS	VM12228-02	Method of Disks,Simpson
MRUS	VM12228-03	Gibson

B.31. CID (12229) Area Methods

CSD	CV	Code Meaning
DCM	125210	Area by Pressure Half-Time
DCM	125212	Continuity Equation
DCM	125213	Continuity Equation by Mean Velocity
DCM	125214	Continuity Equation by Peak Velocity
DCM	125215	Continuity Equation by Velocity Time Integral
DCM	125216	Proximal Isovelocity Surface Area
DCM	125220	Planimetry

B.32. CID (12230) Gradient Methods

CSD	CV	Code Meaning
DCM	125217	Full Bernoulli
DCM	125218	Simplified Bernoulli

B.33. CID (12231) Volume Flow Methods

CSD	CV	Code Meaning
DCM	125219	Doppler Volume Flow
DCM	125216	Proximal Isovelocity Surface Area

B.34. CID (12232) Myocardium Mass Methods

CSD	CV	Code Meaning
DCM	125221	Left Ventricle Mass by M-mode
DCM	125222	Left Ventricle Mass by Truncated Ellipse

B.35. CID (12233) Cardiac Phase

CSD	CV	Code Meaning
SRT	F-32020	Systole
SRT	F-32010	Diastole
SRT	F-32011	End Diastole
DCM	109070	End Systole

B.36. CID (12234) Respiration Phase

CSD	CV	Code Meaning
SRT	F-20010	During Inspiration
SRT	F-20020	During Expiration

B.37. CID (12239) Cardiac Output Properties

CSD	CV	Code Meaning
SRT	F-32120	Stroke Volume
SRT	F-32100	Cardiac Output
SRT	F-32110	Cardiac Index
SRT	F-00078	Stroke Index

B.38. CID (12240) Left Ventricle Area

CSD	CV	Code Meaning
SRT	G-0374	Left Ventricular Systolic Area

SRT	G-0375	Left Ventricular Diastolic Area
SRT	G-0379	Left Ventricle Epicardial Diastolic Area, psax pap view
MRUS	M12240-01	Left Ventricle Endocardiac Diastolic Area, psax pap view

B.39. CID (90000) Pericardial disease

CSD	**CV**	**Code Meaning**
MRUS	C90000-01	Pericard Effusion at end-diastole
MRUS	C90000-02	Pericard Effusion at end-systole

B.40. Mapping between Modality measurements and DICOM Concepts.

B.40.1. Left Ventricle Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
LVOT HR	8867-4,LN,Heart rate	
LVIDd(2D)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode;
LVIDd Cube(2D)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
LVIDd Teich(2D)		

LVIDd(BP Ellipse)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
LVIDd(M)	29436-3,LN,Left Ventricle Internal End Diastolic Dimension	ImageMode = G-0394,SRT,M Mode;
LVIDs(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode;
LVIDs Cube(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
LVIDs Teich(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
LVIDs Gibson(2D)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
LVIDs Cube(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
LVIDs Teich(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
LVIDs Gibson(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
LVIDs(BP Ellipse)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
LVIDs(M)	29438-9,LN,Left Ventricle Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode;
FS(Cube-M)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
FS(Teich-M)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
FS(Gibson-M)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
FS(Cube-2D)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
FS(Teich-2D)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
FS(Gibson-2D)	18051-3,LN,Left Ventricular Fractional Shortening	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
IVSd(2D)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode;
IVSd(LV Mass Cube-2D)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode;

IVSd(LV Mass Cube-M)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
IVSd(M)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =
IVSd Teich(2D)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
IVSd Teich(M)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
IVSd Cube(2D)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
IVSd Cube(M)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
IVSd Gibson(2D)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
IVSd Gibson(M)	18154-5,LN,Interventricular Septum Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
IVSd/LVPWd(2D)	18155-2,LN,Interventricular Septum to Posterior Wall Thickness Ratio	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-03A2,SRT,2D mode;
IVSs/LVPWs(2D)	18155-2,LN,Interventricular Septum to Posterior Wall Thickness Ratio	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-03A2,SRT,2D mode;
IVSd/LVPWd(M)	18155-2,LN,Interventricular Septum to Posterior Wall Thickness Ratio	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-0394,SRT,M Mode;
IVSs/LVPWs(M)	18155-2,LN,Interventricular Septum to Posterior Wall Thickness Ratio	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-0394,SRT,M Mode;
IVS%(2D)	18054-7,LN,Interventricular Septum % Thickening	ImageMode = G-03A2,SRT,2D mode;
IVS%(M)	18054-7,LN,Interventricular Septum % Thickening	ImageMode = G-0394,SRT,M Mode;
IVSs(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode;
IVSs(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode;
IVSs Teich(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
IVSs Teich(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
IVSs Cube(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method

IVSs Cube(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
IVSs Gibson(2D)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
IVSs Gibson(M)	18158-6,LN,Interventricular Septum Systolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
LVPW%(2D)	18053-9,LN,Left Ventricle Posterior Wall % Thickening	ImageMode = G-03A2,SRT,2D mode;
LVPW%(M)	18053-9,LN,Left Ventricle Posterior Wall % Thickening	ImageMode = G-0394,SRT,M Mode;
LVLd apical(Mod.Simpson)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
LVLd(A2C)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
LVLd(A4C)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVLd apical(SP Ellipse)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
LVLd apical(Bullet)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
LVLd apical(LV Mass A-L)	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; Method =125205,DCM,Area-Length Single Plane
LVLd2i	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
LVLd4i	18077-8,LN,Left Ventricle diastolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
LVLs apical(Mod.Simpson)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode;
LVLs(A2C)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125226,DCM,Single Plane Ellipse

LVLs(A4C)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125226,DCM,Single Plane Ellipse
LVLs apical(SP Ellipse)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode;
LVLs apical(Bullet)	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode;
LVLs2i	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
LVLs4i	18076-0,LN,Left Ventricle systolic major axis	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
LVPWs(2D)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode;
LVPWs(M)	18156-0,LN,Left Ventricle Posterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode;

LVPWd(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode;
LVPWd Cube(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
LVPWd Cube(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
LVPWd Teich(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
LVPWd Teich(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
LVPWd Gibson(2D)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
LVPWd Gibson(M)	18152-9,LN,Left Ventricle Posterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode; Method =VM12228

rd2i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
rd4i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =F-32011,SRT,End Diastole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
rs2i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
rs4i	M12222-06,MRUS,Flow Radius	CardiacCyclePoint =109070,SRT,End Systole; ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
LV Area(s)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode = G-03A2,SRT,2D mode;
LVAs apical(SP Ellipse)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode = G-03A2,SRT,2D mode; ImageView = G-0395,SRT,Apical long axis;
LVAs sax MV(Mod.Simpson)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level;
LVAs sax PM	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level;
LVAs(A2C)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAs(A4C)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAs sax MV(BP Ellipse)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =125211,DCM,Biplane Ellipse

LVAs sax MV(Bullet)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =VM12228-01,MRUS,Bullet
LVAs apical(BP Ellipse)	G-0374,SRT,Left Ventricular Systolic Area	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
LV Area(d)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode;
LVAd apical(SP Ellipse)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-0395,SRT,Apical long axis;
LVAd sax MV(Mod.Simpson)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level;
LVAd sax PM	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level;
LVAd(A2C)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAd(A4C)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVAd sax MV(BP Ellipse)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =125211,DCM,Biplane Ellipse
LVAd sax MV(Bullet)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039A,SRT,Parasternal short axis at the Mitral Valve level; Method =VM12228-01,MRUS,Bullet
LVAd apical(BP Ellipse)	G-0375,SRT,Left Ventricular Diastolic Area	ImageMode =G-03A2,SRT,2D mode; ImageView = G-0395,SRT,Apical long axis; Method =125211,DCM,Biplane Ellipse
LVAd sax Epi(LV Mass T-E)	G-0379,SRT,Left Ventricle Epicardial Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse

LVAd sax Epi(LV Mass A-L)	G-0379,SRT,Left Ventricle Epicardial Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125205,DCM,Area-Length Single Plane
LVAd sax Endo(LV Mass T-E)	M12240-01,MRUS,Left Ventricle Endocardiac Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LVAd sax Endo(LV Mass A-L)	M12240-01,MRUS,Left Ventricle Endocardiac Diastolic Area, psax pap view	ImageMode =G-03A2,SRT,2D mode; ImageView = G-039B,SRT,Parasternal short axis at the Papillary Muscle level; Method =125205,DCM,Area-Length Single Plane
EDV(SP Ellipse)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
EDV(BP Ellipse)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
EDV(Bullet)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
EDV(Mod.Simpson)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
EDV(Simp SP-A2C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125208,DCM,Method of Disks, Single Plane
EDV(Simpson BP)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
EDV(Simp BP-A2C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
EDV(Simp BP-A4C)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
EDV(Cube-M)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
EDV(Teich-M)	18026-5,LN,Left Ventricular End Diastolic Volume	ImageMode =G-0394,SRT,M Mode; Method =125209,DCM,Teichholz

Mindray DP-50 Series Digital Ultrasonic Diagnostic Imaging System

ESV(Gibson-M)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
ESV(Cube-2D)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
ESV(Teich-2D)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
ESV(Gibson-2D)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
ESV(Simp SP-A4C)	18148-7,LN,Left Ventricular End Systolic Volume	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
EF(SP Ellipse)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
EF(BP Ellipse)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
EF(Bullet)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
EF(Mod.Simpson)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
EF(A2C)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
EF(Simpson BP)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
EF2(Simpson BP)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
EF4(Simpson BP)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
EF(Cube-M)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
EF(Teich-M)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-0394,SRT,M Mode; Method =125209,DCM,Teichholz

EF(Gibson-M)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
EF(Cube-2D)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
EF(Teich-2D)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz
EF(Gibson-2D)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
EF(A4C)	18043-0,LN,Left Ventricular Ejection Fraction	ImageMode =G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVOT Area	G-038E,SRT,Cardiovascular Orifice Area	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(2D)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(M)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-0394,SRT,M Mode;
LVOT Diam(MVA VTI)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(AVA VTI)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Diam(AVA Vmax)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
LVOT Vmax	11726-7,LN,Peak Velocity	
LVOT Vmax(LVOT VTI)	11726-7,LN,Peak Velocity	
LVOT Vmean	20352-1,LN,Mean Velocity	
LVOT PGmax	20247-3,LN,Peak Gradient	
LVOT PGmax(LVOT VTI)	20247-3,LN,Peak Gradient	
LVOT PGmean	20256-4,LN,Mean Gradient	
LVOT VTI	20354-7,LN,Velocity Time Integral	
LVOT VTI(MVA VTI)	20354-7,LN,Velocity Time Integral	
LVOT VTI(AVA VTI)	20354-7,LN,Velocity Time Integral	
LVOT AccT	20168-1,LN,Acceleration Time	
LVOT	M12222-01,MRUS, Angle	
LVOT Acc Slope	M12222-02,MRUS, Acceleration Slope	

LV Mass(Cube-M)	18087-7,LN,Left Ventricle Mass	ImageMode =G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
LV Mass(T-E)	18087-7,LN,Left Ventricle Mass	ImageMode =G-03A2,SRT,2D mode; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LV Mass(A-L)	18087-7,LN,Left Ventricle Mass	ImageMode =G-03A2,SRT,2D mode; Method =125205,DCM,Area-Length Single Plane
LV Mass(Cube-2D)	18087-7,LN,Left Ventricle Mass	ImageMode =G-03A2,SRT,2D mode;
IVRT	18071-1,LN,Left Ventricular Isovolumic Relaxation Time	
IVCT	G-037E,SRT,Left Ventricular Isovolumic Contraction Time	
LVIMP(M)	G-037F,SRT,Left Ventricular Index of Myocardial Performance	ImageMode =G-0394,SRT,M Mode;
LVIMP(Doppler)	G-037F,SRT,Left Ventricular Index of Myocardial Performance	
LVPEP(M)	M12203-01,MRUS,Left Ventricle Pre-Ejection Period	ImageMode =G-0394,SRT,M Mode;
LVPEP(Doppler)	M12203-01,MRUS,Left Ventricle Pre-Ejection Period	
LVET(M)	M12203-02,MRUS,Left Ventricle Ejection Time	ImageMode =G-0394,SRT,M Mode;
LVET(Doppler)	M12203-02,MRUS,Left Ventricle Ejection Time	
LVET LVIMP(M)	M12203-02,MRUS,Left Ventricle Ejection Time	ImageMode =G-0394,SRT,M Mode;
LVET LVIMP(Doppler)	M12203-02,MRUS,Left Ventricle Ejection Time	
LV Mass-I(Cube-M)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-0394,SRT,M Mode; Method =125221,DCM,Left Ventricle Mass by M-mode
LV Mass-I(T-E)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-03A2,SRT,2D mode; Method =125222,DCM,Left Ventricle Mass by Truncated Ellipse
LV Mass-I(A-L)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-03A2,SRT,2D mode; Method =125205,DCM,Area-Length Single Plane

LV Mass-I(Cube-2D)	C12203-01,MRUS,Left ventricular Mass Weight Index	ImageMode =G-03A2,SRT,2D mode;
LVPEP/ET(M)	C12203-02,MRUS,Left Ventricle Pre-Ejection Period to Ejection Time Ratio	ImageMode =G-0394,SRT,M Mode;
LVPEP/ET(Doppler)	C12203-02,MRUS,Left Ventricle Pre-Ejection Period to Ejection Time Ratio	
LVOT SV	F-32120,SRT,Stroke Volume	
SV(SP Ellipse)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
SV(BP Ellipse)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
SV(Bullet)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
SV(Mod.Simpson)	F-32120,SRT,Stroke Volume	ImageMode =G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
SV(A2C)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
SV(Simpson BP)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
SV2(Simpson BP)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
SV4(Simpson BP)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
SV(Cube-M)	F-32120,SRT,Stroke Volume	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
SV(Teich-M)	F-32120,SRT,Stroke Volume	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
SV(Gibson-M)	F-32120,SRT,Stroke Volume	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
SV(Cube-2D)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
SV(Teich-2D)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz

SV(Gibson-2D)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
SV(A4C)	F-32120,SRT,Stroke Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVOT CO	F-32100,SRT,Cardiac Output	
CO(SP Ellipse)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
CO(BP Ellipse)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
CO(Bullet)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
CO(Mod.Simpson)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
CO(A2C)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
CO(Simpson BP)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
CO2(Simpson BP)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
CO4(Simpson BP)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane
CO(Cube-M)	F-32100,SRT,Cardiac Output	ImageMode = G-0394,SRT,M Mode; Method =125206,DCM,Cube Method
CO(Teich-M)	F-32100,SRT,Cardiac Output	ImageMode = G-0394,SRT,M Mode; Method =125209,DCM,Teichholz
CO(Gibson-M)	F-32100,SRT,Cardiac Output	ImageMode = G-0394,SRT,M Mode; Method =VM12228-03,MRUS,Gibson
CO(Cube-2D)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125206,DCM,Cube Method
CO(Teich-2D)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =125209,DCM,Teichholz

CO(Gibson-2D)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
CO(A4C)	F-32100,SRT,Cardiac Output	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane
LVOT CI	F-32110,SRT,Cardiac Index	
CI(SP Ellipse)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125226,DCM,Single Plane Ellipse
CI(BP Ellipse)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125211,DCM,Biplane Ellipse
CI(Bullet)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-01,MRUS,Bullet
CI(Mod.Simpson)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-02,MRUS,Method of Disks,Simpson
CI(A2C)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125208,DCM,Method of Disks, Single Plane
CI(Simpson BP)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; Method =125207,DCM,Method of Disks, Biplane
CI2(Simpson BP)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method =125207,DCM,Method of Disks, Biplane
CI4(Simpson BP)	F-32110,SRT,Cardiac Index	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125207,DCM,Method of Disks, Biplane

SI(Gibson-2D)	F-00078,SRT,Stroke Index	ImageMode = G-03A2,SRT,2D mode; Method =VM12228-03,MRUS,Gibson
SI(A4C)	F-00078,SRT,Stroke Index	G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method =125208,DCM,Method of Disks, Single Plane

B.40.2. Right Ventricle Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
RVDd(2D)	20304-2,LN,Right Ventricular Internal Diastolic Dimension	ImageMode = G-03A2,SRT,2D mode;
RVDd(M)	20304-2,LN,Right Ventricular Internal Diastolic Dimension	ImageMode = G-0394,SRT,M Mode;
RVDs(2D)	20305-9,LN,Right Ventricular Internal Systolic Dimension	ImageMode = G-03A2,SRT,2D mode;
RVDs(M)	20305-9,LN,Right Ventricular Internal Systolic Dimension	ImageMode = G-0394,SRT,M Mode;
RVIMP	G-0381,SRT,Right Ventricular Index of Myocardial Performance	
RVSP	G-0380,SRT,Right Ventricular Peak Systolic Pressure	
RVAWd(2D)	18153-7,LN,Right Ventricular Anterior Wall Diastolic Thickness	ImageMode = G-03A2,SRT,2D mode;
RVAWd(M)	18153-7,LN,Right Ventricular Anterior Wall Diastolic Thickness	ImageMode = G-0394,SRT,M Mode;
RVAWs(2D)	18157-8,LN,Right Ventricular Anterior Wall Systolic Thickness	ImageMode = G-03A2,SRT,2D mode;
RVAWs(M)	18157-8,LN,Right Ventricular Anterior Wall Systolic Thickness	ImageMode = G-0394,SRT,M Mode;
RV Major	M12204-01,MRUS,Right ventricular Major	ImageMode = G-03A2,SRT,2D mode;
RV Minor	M12204-02,MRUS,Right ventricular Minor	ImageMode = G-03A2,SRT,2D mode;
RV Area(d)	M12204-03,MRUS,Right ventricular Area at end-diastole	ImageMode = G-03A2,SRT,2D mode;
RV Area(s)	M12204-04,MRUS,Right ventricular Area at end-systole	ImageMode = G-03A2,SRT,2D mode;
RVPEP(M)	M12204-05,MRUS,Right Ventricle Pre-Ejection Period	
RVPEP(Doppler)	M12204-05,MRUS,Right Ventricle Pre-Ejection Period	

LAA(A2C)	17977-0,LN,Left Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method = 125205,DCM,Area-Length Single Plane
LAA(A4C)	17977-0,LN,Left Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method = 125205,DCM,Area-Length Single Plane
LA Vol(A-L)	G-0383,SRT,Left Atrium Systolic Volume	ImageMode = G-03A2,SRT,2D mode; Method = 125205,DCM,Area-Length Single Plane
LA Vol(A2C)	G-0383,SRT,Left Atrium Systolic Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19B,SRT,Apical two chamber; Method = 125208,DCM,Method of Disks, Single Plane
LA Vol(A4C)	G-0383,SRT,Left Atrium Systolic Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method = 125208,DCM,Method of Disks, Single Plane
LA Major	M12205-01,MRUS,Left atrium Major	ImageMode = G-03A2,SRT,2D mode;
LA Minor	M12205-02,MRUS,Left atrium Minor	ImageMode = G-03A2,SRT,2D mode;
LeftA.AR/LA.M	C12205-01,MRUS,Aortic Root to Left Atrium Ratio	

B.40.4. Right Atrium Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
RAP	18070-3,LN,Right Atrium Systolic Pressure	
RA Area	17988-7,LN,Right Atrium Systolic Area	ImageMode = G-03A2,SRT,2D mode;
RA Major	M12206-01,MRUS,Right atrium Major	ImageMode = G-03A2,SRT,2D mode;
RA Minor	M12206-02,MRUS,Right atrium Minor	ImageMode = G-03A2,SRT,2D mode;
RA Vol(A4C)	M12206-03,MRUS,Right atrium Volume	ImageMode = G-03A2,SRT,2D mode; ImageView = G-A19C,SRT,Apical four chamber; Method = 125208,DCM,Method of Disks, Single Plane

B.40.5. Aortic Valve Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
ACS(2D)	17996-0,LN,Aortic Valve Cusp Separation	ImageMode = G-03A2,SRT,2D mode;
ACS(M)	17996-0,LN,Aortic Valve Cusp Separation	ImageMode = G-0394,SRT,M Mode;
AV AccT/ET	G-0382,SRT,Ratio of Aortic Valve Acceleration Time to Ejection Time	
AV HR	8867-4,LN,Heart rate	
AR Flow	33878-0,LN,Volume Flow	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AR Flow Rate	34141-2,LN,Peak Instantaneous Flow Rate	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AVA	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT,Antegrade Flow; ImageMode = G-03A2,SRT,2D mode; Method =125220,DCM,Planimetry
AVA(VTI)	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT,Antegrade Flow; Method =125215,DCM,Continuity Equation by Velocity Time Integral
AV Diam(2D)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode = G-03A2,SRT,2D mode;
AV Diam(Qp/Qs)	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode = G-03A2,SRT,2D mode;
AR Fraction	G-0390,SRT,Regurgitant Fraction	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AR Ved	11653-3,LN,End Diastolic Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow
AV Vmax	11726-7,LN,Peak Velocity	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Vmax	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR Vmax(AR VTI)	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR Vmax(AR PHT)	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR Vmax(PISA AR)	11726-7,LN,Peak Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AV Vmax(AV VTI)	11726-7,LN,Peak Velocity	Flow Direction = R-42047,SRT,Antegrade Flow;

AV Vmean	20352-1,LN,Mean Velocity	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Vmean	20352-1,LN,Mean Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV PGmax	20247-3,LN,Peak Gradient	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PGmax	20247-3,LN,Peak Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV PGmax(AV VTI)	20247-3,LN,Peak Gradient	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PGmax(AR VTI)	20247-3,LN,Peak Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR PGmax(AR PHT)	20247-3,LN,Peak Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV PGmean	20256-4,LN,Mean Gradient	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PGmean	20256-4,LN,Mean Gradient	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV VTI	20354-7,LN,Velocity Time Integral	Flow Direction = R-42047,SRT,Antegrade Flow;
AR VTI	20354-7,LN,Velocity Time Integral	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV VTI(Qp/Qs)	20354-7,LN,Velocity Time Integral	Flow Direction = R-42047,SRT,Antegrade Flow;
AR VTI(PISA AR)	20354-7,LN,Velocity Time Integral	Flow Direction = R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
AV VTI(AVA VTI)	20354-7,LN,Velocity Time Integral	Flow Direction = R-42047,SRT,Antegrade Flow;
AR PHT	20280-4,LN,Pressure Half-Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV AccT	20168-1,LN,Acceleration Time	Flow Direction = R-42047,SRT,Antegrade Flow;
AV DecT	20217-6,LN,Deceleration Time	Flow Direction = R-42047,SRT,Antegrade Flow;
AR DcT	20217-6,LN,Deceleration Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR DecT	20217-6,LN,Deceleration Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV Acc Slope	M12222-02,MRUS,Acceleration Slope	Flow Direction = R-42047,SRT,Antegrade Flow;
AR Rad	M12222-06,MRUS,Flow Radius	Flow Direction = R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
AR Als.Vel	M12222-05,MRUS,Aliasing Velocity	Flow Direction = R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
AR Time	M12222-04,MRUS,Time	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AR DcR	M12222-03,MRUS,Deceleration Rate	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV	M12222-01,MRUS,Angle	Flow Direction = R-42047,SRT,Antegrade Flow;
AR	M12222-01,MRUS,Angle	Flow Direction = R-42E61,SRT,Regurgitant Flow;
AV SV	F-32120,SRT,Stroke Volume	
AV CO	F-32100,SRT,Cardiac Output	

AV CI	F-32110,SRT,Cardiac Index	
AV SI	F-00078,SRT,Stroke Index	
PISA	M12222-09,MRUS, Effective Regurgitant Orifice Area	

B.40.6. Mitral Valve Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
MV A Vel	17978-8 LN Mitral Valve A-Wave Peak Velocity	Image Mode = G-0394,SRT,M Mode
MV A Vel	17978-8,LN,Mitral Valve A-Wave Peak Velocity	
MV A Vel(MV A VTI)	17978-8,LN,Mitral Valve A-Wave Peak Velocity	
MV A Vel(MV E/A)	17978-8,LN,Mitral Valve A-Wave Peak Velocity	
MV E Vel	18037-2,LN,Mitral Valve E-Wave Peak Velocity	
MV E Vel(MV E VTI)	18037-2,LN,Mitral Valve E-Wave Peak Velocity	
MV E Vel(MV E/A)	18037-2,LN,Mitral Valve E-Wave Peak Velocity	
MV E/A	18038-0,LN,Mitral Valve E to A Ratio	
MV E/A(MV E/A)	18038-0,LN,Mitral Valve E to A Ratio	
MV AccT/DecT	G-0386,SRT,Mitral Valve AT/DT Ratio	
MV E-F Slope	18040-6,LN,Mitral Valve E-F Slope by M-Mode	ImageMode = G-0394,SRT,M Mode ;
EPSS(2D)	18036-4,LN,Mitral Valve EPSS, E wave	ImageMode = G-03A2,SRT,2D mode ;
EPSS(M)	18036-4,LN,Mitral Valve EPSS, E wave	ImageMode = G-0394,SRT,M Mode ;
MV A Dur	G-0385,SRT,Mitral Valve A-Wave Duration	
MV C-O dur(M)	G-0387,SRT,Mitral Valve Closure to Opening Time	ImageMode = G-0394,SRT,M Mode ;
MV C-O dur(Doppler)	G-0387,SRT,Mitral Valve Closure to Opening Time	
dP/dt	18035-6,LN,Mitral Regurgitation Dp/dt derived from Mitral Reg. velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MCS(2D)	M12207-01,MRUS,Mitral valve cusp separate distance	ImageMode = G-03A2,SRT,2D mode ;
MCS(M)	M12207-01,MRUS,Mitral valve cusp separate distance	ImageMode = G-0394,SRT,M Mode ;
MV D-E Slope	M12207-02,MRUS,Mitral Valve D-E Slope	ImageMode = G-0394,SRT,M Mode ;
MV A Amp	M12207-03,MRUS,Amplitude of the A wave	ImageMode = G-0394,SRT,M Mode ;

MV E Amp	M12207-04,MRUS,Amplitude of the E wave	ImageMode = G-0394,SRT,M Mode ;
MV DE	M12207-05,MRUS,Amplitude from D Point to E Point	ImageMode = G-0394,SRT,M Mode ;
MV E PG	M12207-06,MRUS,Mitral Valve E-wave Pressure Gradient	
MV A PG	M12207-07,MRUS,Mitral Valve A-wave Pressure Gradient	
MV E VTI	M12207-08,MRUS,E wave Velocity Time Integral	Flow Direction =R-42047,SRT,Antegrade Flow;
MV A VTI	M12207-09,MRUS,A wave Velocity Time Integral	Flow Direction =R-42047,SRT,Antegrade Flow;
MV E Dur	M12207-10,MRUS,Mitral Valve E-Wave Duration	
Sa(medial)	M12207-11,MRUS,Systolic Velocity of the Mitral Annulus(medial)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea(medial)	M12207-12,MRUS,Early diastolic velocity of the mitral annulus(medial)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Aa(medial)	M12207-13,MRUS,Late diastolic velocity of the mitral annulus(medial)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea/Aa(medial)	M12207-14,MRUS,Early diastolic velocity to Late diastolic velocity Ratio	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ata(medial)	M12207-15,MRUS,Acceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ara(medial)	M12207-16,MRUS,Acceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dta(medial)	M12207-17,MRUS,Deceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dra(medial)	M12207-18,MRUS,Deceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Sa(lateral)	M12207-19,MRUS,Systolic Velocity of the Mitral Annulus(lateral)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;

Ea(lateral)	M12207-20,MRUS,Early diastolic velocity of the mitral annulus(lateral)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Aa(lateral)	M12207-21,MRUS,Late diastolic velocity of the mitral annulus(lateral)	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ea/Aa(lateral)	M12207-22,MRUS,Early diastolic velocity to Late diastolic velocity Ratio	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ata(lateral)	M12207-23,MRUS,Acceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Ara(lateral)	M12207-24,MRUS,Acceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dta(lateral)	M12207-25,MRUS,Deceleration Time of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
Dra(lateral)	M12207-26,MRUS,Deceleration Rate of Early diastolic velocity	ImageMode = IM12224-01,MRUS,Tissue Doppler Imaging;
MS Rad	M12207-27,MRUS,Mitral Stenosis Radius	ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MS Als.Vel	M12207-28,MRUS,Mitral Stenosis Aliasing Velocity	ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MS Vmax	M12207-29,MRUS,Mitral Stenosis Maximum Velocity	
MS Vmax(PISA MS)	M12207-29,MRUS,Mitral Stenosis Maximum Velocity	Method = 125216,DCM,Proximal Isovelocity Surface Area
MS Area	M12207-30,MRUS,Mitral Stenosis Area	Method = 125216,DCM,Proximal Isovelocity Surface Area
MS Pgmax	C12207-01,MRUS,Mitral Stenosis Maximum Pressure Gradient	
MV HR	8867-4,LN,Heart rate	

MR Flow	33878-0,LN,Volume Flow	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MR Flow Rate	34141-2,LN,Peak Instantaneous Flow Rate	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MVA	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT,Antegrade Flow; ImageMode = G-03A2,SRT,2D mode; Method = 125220,DCM,Planimetry
MVA(PHT)	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT,Antegrade Flow; Method = 125210,DCM,Area by Pressure Half-Time
MVA(VTI)	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT,Antegrade Flow; Method = 125215,DCM,Continuity Equation by Velocity Time Integral
MV Diam	G-038F,SRT,Cardiovascular Orifice Diameter	Flow Direction =R-42047,SRT,Antegrade Flow; ImageMode = G-03A2,SRT,2D mode;
MR Fraction	G-0390,SRT,Regurgitant Fraction	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MV Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
MR Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = G-03A2,SRT,2D mode;
MV Vmax(MV PHT)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
MV Vmax(MV VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;

MR Vmax(MR VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MR Vmax(PISA MR)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MV Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
MR Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MV Pgmax	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
MR Pgmax	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MV Pgmean	20256-4,LN,Mean Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
MR Pgmean	20256-4,LN,Mean Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MV VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42047,SRT, Antegrade Flow;
MR VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MV VTI(MVA VTI)	20354-7,LN,Velocity Time Integral	Flow Direction =R-42047,SRT, Antegrade Flow;
MR VTI(PISA MR)	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
MV PHT	20280-4,LN,Pressure Half-Time	Flow Direction =R-42047,SRT, Antegrade Flow;
MV AccT	20168-1,LN,Acceleration Time	Flow Direction =R-42047,SRT, Antegrade Flow;
MV DecT	20217-6,LN,Deceleration Time	Flow Direction =R-42047,SRT, Antegrade Flow;
MV Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction =R-42047,SRT, Antegrade Flow;
MV Acc Slope	M12222-02,MRUS,Acceleration Slope	Flow Direction =R-42047,SRT, Antegrade Flow;
dt	M12222-04,MRUS,Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;

MR Rad	M12222-06,MRUS,Flow Radius	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
MR Als.Vel	M12222-05,MRUS,Aliasing Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
MV	M12222-01,MRUS,Angle	Flow Direction =R-42047,SRT,Antegrade Flow;
MR	M12222-01,MRUS,Angle	Flow Direction =R-42E61,SRT,Regurgitant Flow;
MV SV	F-32120,SRT,Stroke Volume	
MV CO	F-32100,SRT,Cardiac Output	
MV CI	F-32110,SRT,Cardiac Index	
MV SI	F-00078,SRT,Stroke Index	
E/Ea	M12207-35,MRUS,MV E/Ea	
PISA	M12222-09,MRUS, Effective Regurgitant Orifice Area	

B.40.7. Pulmonic Valve Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
PV	M12222-01,MRUS,Angle	Flow Direction =R-42047,SRT,Antegrade Flow;
PR	M12222-01,MRUS,Angle	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV HR	8867-4,LN,Heart rate	
PR Flow	33878-0,LN,Volume Flow	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
PR Flow Rate	34141-2,LN,Peak Instantaneous Flow Rate	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
PV Diam	G-038F,SRT,Cardiovascular Orifice Diameter	Flow Direction =R-42047,SRT,Antegrade Flow; ImageMode = G-03A2,SRT,2D mode;
PV Diam(Qp/Qs)	G-038F,SRT,Cardiovascular Orifice Diameter	Flow Direction =R-42047,SRT,Antegrade Flow; ImageMode = G-03A2,SRT,2D mode;
PR Fraction	G-0390,SRT,Regurgitant Fraction	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area

PR Ved	11653-3,LN,End Diastolic Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR Ved(PAEDP)	11653-3,LN,End Diastolic Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
PR Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV Vmax(PV VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
PR Vmax(PR VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR Vmax(PR PHT)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR Vmax(PISA PR)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
PR Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV PGmax	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT,Antegrade Flow;
PR PGmax	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV PGmax(PV VTI)	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
PR PGmax(PR VTI)	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR PGmax(PR PHT)	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV PGmean	20256-4,LN,Mean Gradient	Flow Direction =R-42047,SRT,Antegrade Flow;
PR PGmean	20256-4,LN,Mean Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42047,SRT,Antegrade Flow;
PR VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV VTI(Qp/Qs)	20354-7,LN,Velocity Time Integral	Flow Direction =R-42047,SRT,Antegrade Flow;
PR VTI(PISA PR)	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR PHT	20280-4,LN,Pressure Half-Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV AccT	20168-1,LN,Acceleration Time	Flow Direction =R-42047,SRT,Antegrade Flow;
PR DecT	20217-6,LN,Deceleration Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV Acc Slope	M12222-02,MRUS,Acceleration Slope	Flow Direction =R-42047,SRT,Antegrade Flow;
PR Rad	M12222-06,MRUS,Flow Radius	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
PR Als.Vel	M12222-05,MRUS,Aliasing Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
PR PGed	M12222-08,MRUS,Presure Gradient at end-Diastole	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PR PGed(PAEDP)	M12222-08,MRUS,Presure Gradient at end-Diastole	Flow Direction =R-42E61,SRT,Regurgitant Flow;
PV SV	F-32120,SRT,Stroke Volume	

PV CO	F-32100,SRT,Cardiac Output	
PV CI	F-32110,SRT,Cardiac Index	
PV SI	F-00078,SRT,Stroke Index	
PISA	M12222-09,MRUS, Effective Regurgitant Orifice Area	

B.40.8. Tricuspid Valve Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
TV E Vel	18031-5,LN,Tricuspid Valve E Wave Peak Velocity	
TV E Vel(TV E/A)	18031-5,LN,Tricuspid Valve E Wave Peak Velocity	
TV A Vel	18030-7,LN,Tricuspid Valve A Wave Peak Velocity	
TV A Vel(TV E/A)	18030-7,LN,Tricuspid Valve A Wave Peak Velocity	
TV E/A	18039-8,LN,Tricuspid Valve E to A Ratio	
TV E/A(TV E/A)	18039-8,LN,Tricuspid Valve E to A Ratio	
TV C-O dur	G-0389,SRT,Tricuspid Valve Closure to Opening Time	
TV	M12222-01,MRUS,Angle	Flow Direction =R-42047,SRT,Antegrade Flow;
TR	M12222-01,MRUS,Angle	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV HR	8867-4,LN,Heart rate	
TR Flow	33878-0,LN,Volume Flow	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TR Flow Rate	34141-2,LN,Peak Instantaneous Flow Rate	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TVA	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT, Antegrade Flow; ImageMode = G-03A2,SRT,2D mode; Method = 125220,DCM,Planimetry
TVA(PHT)	G-038E,SRT,Cardiovascular Orifice Area	Flow Direction =R-42047,SRT, Antegrade Flow; Method = 125210,DCM,Area by Pressure Half-Time

TV Diam	G-038F,SRT,Cardiovascular Orifice Diameter	Flow Direction =R-42047,SRT, Antegrade Flow; ImageMode = G-03A2,SRT,2D mode;
TR Fraction	G-0390,SRT,Regurgitant Fraction	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TV Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Vmax	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV Vmax(TV PHT)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TV Vmax(TV VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Vmax(TR VTI)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR Vmax(PISA TR)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method = 125216,DCM,Proximal Isovelocity Surface Area
TR Vmax(RVSP)	11726-7,LN,Peak Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Vmean	20352-1,LN,Mean Velocity	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV PGmax(TV PHT)	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TV PGmax(TV VTI)	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TV PGmax	20247-3,LN,Peak Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TR PGmax	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR PGmax(TR VTI)	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR PGmax(RVSP)	20247-3,LN,Peak Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV PGmean	20256-4,LN,Mean Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TR PGmean	20256-4,LN,Mean Gradient	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42047,SRT, Antegrade Flow;
TR VTI	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TR VTI(PISA TR)	20354-7,LN,Velocity Time Integral	Flow Direction =R-42E61,SRT,Regurgitant Flow; Method =125216,DCM,Proximal Isovelocity Surface Area
TV PHT	20280-4,LN,Pressure Half-Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV AccT	20168-1,LN,Acceleration Time	Flow Direction =R-42047,SRT, Antegrade Flow;
TV DecT	20217-6,LN,Deceleration Time	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV Dec Slope	20216-8,LN,Deceleration Slope	Flow Direction =R-42E61,SRT,Regurgitant Flow;
TV A Dur	M12208-01,MRUS,Tricuspid Valve E-Wave Duration	Flow Direction =R-42047,SRT, Antegrade Flow;

TV E PG	M12208-02,MRUS,Tricuspid Valve E Wave Pressure Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TV A PG	M12208-03,MRUS,Tricuspid Valve A Wave Pressure Gradient	Flow Direction =R-42047,SRT, Antegrade Flow;
TV Acc Slope	M12222-02,MRUS,Acceleration Slope	Flow Direction =R-42047,SRT, Antegrade Flow;
TV AccT/DecT	M12222-07,MRUS,Acceleration Time/Deceleration Time	Flow Direction =R-42047,SRT, Antegrade Flow;
TR Rad	M12222-06,MRUS,Flow Radius	Flow Direction =R-42E61,SRT,Regurgitant Flow; ImageMode = R-409E2, SRT, Doppler Color Flow;
TR Als.Vel	M12222-02,MRUS,Aliasing Velocity	ImageMode = R-409E2, SRT, Doppler Color Flow;
TV SV	F-32120,SRT,Stroke Volume	
TV CO	F-32100,SRT,Cardiac Output	
TV CI	F-32110,SRT,Cardiac Index	
TV SI	F-00078,SRT,Stroke Index	
PISA	M12222-09,MRUS, Effective Regurgitant Orifice Area	

B.40.9. Aorta Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
Ao Diam(2D)	18015-8,LN,Aortic Root Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Diam(M)	18015-8,LN,Aortic Root Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Diam(LA/Ao-2D)	18015-8,LN,Aortic Root Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Diam(LA/Ao-M)	18015-8,LN,Aortic Root Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Arch Diam(2D)	18011-7,LN,Aortic Arch Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Arch Diam(M)	18011-7,LN,Aortic Arch Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Asc Diam(2D)	18012-5,LN,Ascending Aortic Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Asc Diam(M)	18012-5,LN,Ascending Aortic Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Isthmus(2D)	18014-1,LN,Aortic Isthmus Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Isthmus(M)	18014-1,LN,Aortic Isthmus Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Desc Diam(2D)	18013-3,LN,Descending Aortic Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Desc Diam(M)	18013-3,LN,Descending Aortic Diameter	ImageMode = G-0394,SRT,M Mode;
Ao st junct(2D)	M12212-01,MRUS,Aortic Sinotubular junction Diameter	ImageMode = G-03A2,SRT,2D mode;

Ao st junct(M)	M12212-01,MRUS,Aortic Sinotubular junction Diameter	ImageMode = G-0394,SRT,M Mode;
Ao Sinus Diam(2D)	M12212-02,MRUS,Aortic Sinus Diameter	ImageMode = G-03A2,SRT,2D mode;
Ao Sinus Diam(M)	M12212-02,MRUS,Aortic Sinus Diameter	ImageMode = G-0394,SRT,M Mode;
Duct Art Diam	M12212-03,MRUS,Ductus Artery Diameter	ImageMode = G-03A2,SRT,2D mode;
Pre Ductal	M12212-04,MRUS,Previous Ductal Diameter	ImageMode = G-03A2,SRT,2D mode;
LCA	M12212-05,MRUS,Left Coronary Artery Diameter	ImageMode = G-03A2,SRT,2D mode;
RCA	M12212-06,MRUS,Right Coronary Artery Diameter	ImageMode = G-03A2,SRT,2D mode;
AAo Vmax	11726-7,LN,Peak Velocity	
DAo Vmax	11726-7,LN,Peak Velocity	
AAo PGmax	20247-3,LN,Peak Gradient	
DAo PGmax	20247-3,LN,Peak Gradient	

B.40.10. Pulmonary Artery Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
MPA Diam(2D)	18020-8,LN,Main Pulmonary Artery Diameter	ImageMode =G-03A2,SRT,2D mode;
MPA Diam(M)	18020-8,LN,Main Pulmonary Artery Diameter	ImageMode =G-0394,SRT,M Mode;
RPA Diam(2D)	18021-6,LN,Right Pulmonary Artery Diameter	ImageMode =G-03A2,SRT,2D mode;
RPA Diam(M)	18021-6,LN,Right Pulmonary Artery Diameter	ImageMode =G-0394,SRT,M Mode;
LPA Diam(2D)	18019-0,LN,Left Pulmonary Artery Diameter	ImageMode =G-03A2,SRT,2D mode;
LPA Diam(M)	18019-0,LN,Left Pulmonary Artery Diameter	ImageMode =G-0394,SRT,M Mode;
MPA Vmax	G-038A,SRT,Main Pulmonary Artery Peak Velocity	
Post Ductal	M12210-01,MRUS,Posterior ductal Diameter	ImageMode =G-03A2,SRT,2D mode;
PAEDP	C12210-01,MRUS,Pulmonary Artery End Diastolic Pressure	
LPA Vmax	11726-7,LN,Peak Velocity	
RPA Vmax	11726-7,LN,Peak Velocity	
MPA PGmax	20247-3,LN,Peak Gradient	
LPA PGmax	20247-3,LN,Peak Gradient	
RPA PGmax	20247-3,LN,Peak Gradient	

B.40.11. Vena Cava Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***

IVC Diam(Insp)	18006-7,LN,Inferior Vena Cava Diameter	RespiratoryCyclePoint=F-20010,SRT, During Inspiration; ImageMode =G-03A2,SRT,2D mode;
IVC Diam(Expir)	18006-7,LN,Inferior Vena Cava Diameter	RespiratoryCyclePoint=F-20020,SRT, During Expiration; ImageMode =G-03A2,SRT,2D mode;
SVC Diam(Insp)	M12215-01,MRUS,Superior Vena Cava Diameter	RespiratoryCyclePoint=F-20010,SRT, During Inspiration; ImageMode =G-03A2,SRT,2D mode;
SVC Diam(Expir)	M12215-01,MRUS,Superior Vena Cava Diameter	RespiratoryCyclePoint=F-20020,SRT, During Expiration; ImageMode =G-03A2,SRT,2D mode;
IVC Vel(Insp)	M12215-02,MRUS,Inferior Vena Cava Velocity	RespiratoryCyclePoint=F-20010,SRT, During Inspiration;
IVC Vel(Expir)	M12215-02,MRUS,Inferior Vena Cava Velocity	RespiratoryCyclePoint=F-20020,SRT, During Expiration;
SVC Vel(Insp)	M12215-03,MRUS,Superior Vena Cava Velocity	RespiratoryCyclePoint=F-20010,SRT, During Inspiration;
SVC Vel(Expir)	M12215-03,MRUS,Superior Vena Cava Velocity	RespiratoryCyclePoint=F-20020,SRT, During Expiration;
IVC Inspiration PG	C12215-01,MRUS,Inferior Vena Cava Pressure Gradient	RespiratoryCyclePoint=F

PVein S/D	M12214-05,MRUS,Pulmonary Vein Ratio of S-Wave velocity to D-wave velocity	
PVein SF	M12214-06,MRUS,Pulmonary Vein Systolic fraction	

B.40.13. Cardiac Shunt Study Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
Qp/Qs	29462-9,LN,Pulmonary-to-Systemic Shunt Flow Ratio	
Qp-Qs	M12217-01,MRUS,Pulmonary-sub-Systemic Shunt Flow Difference	
PV HR(Qp/Qs)	8867-4,LN,Heart rate	
AV HR(Qp/Qs)	8867-4,LN,Heart rate	
PV SV(Qp/Qs)	F-32120,SRT,Stroke Volume	
PV CO(Qp/Qs)	F-32100,SRT,Cardiac Output	
AV SV(Qp/Qs)	F-32120,SRT,Stroke Volume	
AV CO(Qp/Qs)	F-32100,SRT,Cardiac Output	

B.40.14. Congenital Anomaly of Cardiovascular System Measurements

MODALITY Label	*DICOM Mapping*	*Optional Modifiers*
PDA Diam	M12218-01,MRUS,Patent Ductus Arteriosus Diameter	ImageMode =G-03A2,SRT,2D mode;
PFO Diam	M12218-02,MRUS,Patent Foramen Ovale Diameter	ImageMode =G-03A2,SRT,2D mode;
PDA Vel(d)	M12218-03,MRUS,Patent Ductus Arteriosus Diastolic Velocity	
PDA Vel(s)	M12218-04,MRUS,Patent Ductus Arteriosus Systolic Velocity	
Coarc Pre-Duct	M12218-05,MRUS,Coarctation of Pre-Ductus Velocity	
Coarc Post-Duct	M12218-06,MRUS,Coarctation of Post-Ductus Velocity	
PDA Dias PG	M12218-07,MRUS,Patent Ductus Arteriosus Diastolic Pressure Gradient	
PDA Sys PG	M12218-08,MRUS,Patent Ductus Arteriosus Systolic Pressure Gradient	
Coarc Pre-Duct PG	M12218-09,MRUS,Coarctation of Pre-Ductus Pressure Gradient	
Coarc Post-Duc PG	M12218-10,MRUS,Coarctation of Post-Ductus Pressure Gradient	
VSD Diam	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;

ASD Diam	G-038F,SRT,Cardiovascular Orifice Diameter	ImageMode =G-03A2,SRT,2D mode;
VSD Vmax	11726-7,LN,Peak Velocity	
ASD Vmax	11726-7,LN,Peak Velocity	
VSD PGmax	20247-3,LN,Peak Gradient	
ASD PGmax	20247-3,LN,Peak Gradient	

B.40.15. Pericardial Disease Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
PEd(2D)	C90000-01,MRUS,Pericard Effusion at end-diastole	ImageMode =G-03A2,SRT,2D mode;
PEd(M)	C90000-01,MRUS,Pericard Effusion at end-diastole	ImageMode =G-0394,SRT,M Mode;
PEs(2D)	C90000-02,MRUS,Pericard Effusion at end-systole	ImageMode =G-03A2,SRT,2D mode;
PEs(M)	C90000-02,MRUS,Pericard Effusion at end-systole	ImageMode =G-0394,SRT,M Mode;

B.40.16. Heart Rate Measurements

MODALITY Label	***DICOM Mapping***	***Optional Modifiers***
HR	8867-4 LN Heart rate	Image Mode = G-0394,SRT,M Mode

C. Appendix : Vascular structured reporting template

This appendix lists the DICOM Structured Report (SR) mappings used in the

Vascular Structured Reports of ultrasound system SR files.

The mappings are organized in a manner similar to the DICOM SR Templates as described in PS 3.16 of the DICOM Standard. The Vascular Report mappings follow the DICOM SR Template TID 5100: Vascular Ultrasound Procedure Report, except where noted.

All private code values use the Coding Scheme Designator "MRUS".

C.1. TID (5100) Vascular Ultrasoud Report

This is the template for the root the content tree for the vascular ultrasound procedure report.

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1							

9 > CONTAINS INCLUDE

13	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12104) Extracranial Arteries $AnatomyRatio = DCID (12123) Carotid Ratios	
14	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12109) Lower Extremity Arteries $AnatomyRatio = 8581-1,LN,Tibial/brachial index	
15	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-470 $SectionLaterality = EV (G- $Anatomy = DCID (12109) Lower Extremity Arteries $AnatomyRatio = 8581-1,LN,Tibial/brachial index	
16	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12110) Lower Extremity Veins	

17	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- of $SectionLaterality = EV (G- $Anatomy = DCID (12110) Lower Extremity Veins	
18	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12107) Upper Extremity Arteries	
19	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (12107) Upper Extremity Arteries	
20	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T- $SectionLaterality = EV (G- $Anatomy = DCID (SELFCID-2) Upper Extremity Arteries(unilateral)	

2 > CONTAINS INCLUDE

1

29	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-71019, $SectionLaterality = EV (G- $Anatomy = DCID (12115) Renal Vessels	
30	>	CONTAINS	INCLUDE	DTID (5103) Vascular Ultrasound Section		$SectionScope = DT (T-71019, $SectionLaterality = EV (G- $Anatomy = DCID (12115) Renal Vessels	
31	>	CONTAINS	INCLUDE	DTID (5105) Ultrasound Graft Section			

C.2. TID (1001) Observation Context

This template specifies attributes of observation context that may be defined, extended or replaced at any location in the SR tree.

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1	>	HAS OBS CONTEXT	CODE	EV (121005,DCM,		(121006,DCM,	
2	>	HAS OBS CONTEXT	PNAME	EV (121008,DCM,		Operator from Info	
3	>	HAS OBS CONTEXT	TEXT	EV (121009,DCM, Organiza		Institution Name (0008,0080) of the General Equipment Module	
4	>	HAS OBS CONTEXT	CODE	EV (121010,DCM, Role in the		(121093, DCM, "Sonographer")	

5	>	HAS OBS CONTEXT	CODE	EV (121024, DCM, "Subject Class		(121025, DCM,	
6	>	HAS OBS CONTEXT	PNAME	EV (121029,DCM,		(0010,0010) in Patient Module	
7	>	HAS OBS CONTEXT	DATE	EV (121031,DCM,		Date (0010,0030) in Patient Module	
8	>	HAS OBS CONTEXT	CODE	EV (121032,DCM,		value equivalent to (0010,0040) in Patient Module	
9	>	HAS OBS CONTEXT	NUM	EV (121033,DCM,		(0010,1010) in Patient Study Module	

C.3. TID (5101) Vascular Patient Characteristics

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1			CONTAINER	EV (121118, DCM,			
2	>	CONTAINS	NUM	EV (121033, DCM, "Subject Ag		Units = DCID (7456) Units of Measure for Age	
3	>	CONTAINS	CODE	EV (121032, DCM,		DCID (7455) Sex	
4	>	CONTAINS	NUM	EV (8867-			
5	>	CONTAINS	NUM	EV (F-008EC, SRT,			
6	>	CONTAINS	NUM	EV (F-008ED, SRT, "Diastolic Blood Pressure")			

C.4. TID (5102) Vascular Procedure Summary Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	COMMENT
1			CONTAINER	DT (121111, DCM,			
2	>	CONTAINS	TEXT	DCID (12101) Vascular Summary			

18	>>	CONTAINS	CONTAINER	(FG3495-01, MRUS, Plaque Description)			
19	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
20	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
21	>>	CONTAINS	CONTAINER	(FG3495-02, MRUS, Plaque Area)			
22	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
23	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
24	>	CONTAINS	CONTAINER	(T-45300, SRT, Internal Carotid Artery)			ICA
25	>>	CONTAINS	CONTAINER	(FG3495-01, MRUS, Plaque Description)			
26	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
27	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
28	>>	CONTAINS	CONTAINER	(FG3495-02, MRUS, Plaque Area)			
29	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
30	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
31	>	CONTAINS	CONTAINER	(T-45200,SRT,External Carotid Artery)			ECA
32	>>	CONTAINS	CONTAINER	(FG3495-01, MRUS, Plaque Description)			
33	>>>	CONTAINS	TEXT	(G-A100,SNM3,Right)			
34	>>>	CONTAINS	TEXT	(G-A101,SNM3,Left)			
35	>>	CONTAINS	CONTAINER	(FG3495-02, MRUS, Plaque Area)			

44	>	CONTAINS	TEXT	(T-46010,SRT,Brachiocephalic trunk)			

C.5. TID (5103) Vascular Ultrasound Section

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1			CONTAINER	DT (121070, DCM,			
2	>	HAS CONCEPT MOD	CODE	EV (G-C0E3, SRT,		$SectionScope	
3	>	HAS CONCEPT MOD	CODE	EV (G-C171, SRT,		$SectionLaterality	
4	>	CONTAINS	INCLUDE	DTID (5104) Vascular Measurement Group		$AnatomyGroup = $Anatomy= DCID (12105) Intracranial Cerebral Vessels	
5	>	CONTAINS	INCLUDE	DTID (300) Measurement		$Measurement = $AnatomyRatio	Only for Artery of neck

C.6. TID (5104) Vascular Ultrasound Measurement Group

	NL	Rel with Parent	VT	Concept Name	Used in MODALITY	Value Set Constraint	Comment
1			CONTAINER	$AnatomyGroup			
2	>	HAS CONCEPT MOD	CODE	EV (G-A1F8, SRT,		DCID (12116) Vessel Segment Modifiers	
3	>	HAS CONCEPT	CODE	EV (125101,		DCID (12117) Vessel Branch Modifiers	

		MOD					
4	>	CONTAINS	INCLUDE	DTID (300) Measurement		$Measurement = DCID (12119) Vascular Ultrasound Property $Derivation = DCID (3627) Measurement Type	
5	>>	HAS CONCEPT MOD	CODE	EV (R-4089A,		DCID (12233) Cardiac Phase	
6	>>	HAS CONCEPT MOD	CODE	EV (R-41FFC, period related to		DT (G-A491, SRT, "Post-prandial")	

C.7. CID (12104) Extracranial Arteries

CSD	CV	Code Meaning
SRT	T-45170	Carotid Bulb
SRT	T-45100	Common Carotid Artery
SRT	T-45200	External Carotid Artery
SRT	T-45300	Internal Carotid Artery
SRT	T-46100	Subclavian Artery
SRT	T-45700	Vertebral Artery

C.8. CID (12105) Intracranial Cerebral Vessels

CSD	CV	Code Meaning
SRT	T-45540	Anterior Cerebral Artery
SRT	T-45600	Middle Cerebral Artery
SRT	T-45900	Posterior Cerebral Artery
SRT	T-45320	Posterior Communicating Artery

C.9. CID (12106) Intracranial Cerebral Vessels (unilateral)

CSD	CV	Code Meaning
SRT	T-45800	Basilar Artery
SRT	T-45530	Anterior Communicating Artery

CSD	CV	Code Meaning
MRUS	V12106-01	Basilar Vein

C.10. CID (12107) Upper Extremity Arteries

CSD	CV	Code Meaning
SRT	T-47100	Axillary Artery
SRT	T-47160	Brachial Artery
SRT	T-47300	Radial Artery
SRT	T-46100	Subclavian Artery
SRT	T-47200	Ulnar Artery

C.11. CID (SELFCID-2) Upper Extremity Arteries(unilateral)

CSD	CV	Code Meaning
SRT	T-46010	Innominate Artery

C.12. CID (12108) Upper Extremity Veins

CSD	CV	Code Meaning
SRT	T-49110	Axillary vein
SRT	T-48052	Basilic vein
SRT	T-49350	Brachial vein
SRT	T-49240	Cephalic vein
SRT	T-49340	Radial vein
SRT	T-48330	Subclavian vein
SRT	T-49330	Ulnar vein

C.13. CID (12109) Lower Extremity Arteries

CSD	CV	Code Meaning
SRT	T-46710	Common Iliac Artery
SRT	T-47700	Anterior Tibial Artery
SRT	T-47400	Common Femoral Artery
SRT	T-47741	Dorsalis Pedis Artery
SRT	T-46910	External Iliac Artery
SRT	T-46740	Internal Iliac Artery
SRT	T-47630	Peroneal Artery

C.16. CID (12114) Abdominal Veins (unilateral)

CSD	CV	Code Meaning
SRT	T-48720	Hepatic Vein
SRT	T-48727	Left Hepatic Vein
SRT	T-48725	Right Hepatic Vein
SRT	T-48726	Middle Hepatic Vein
SRT	T-48810	Portal Vein
SRT	T-48710	Inferior Vena Cava
SRT	T-48890	Splenic Vein
SRT	T-48840	Superior Mesenteric Vein
MRUS	V12114-01	Main Portal Vein

C.17. CID (12115) Renal Vessels

CSD	CV	Code Meaning
SRT	T-46600	Renal Artery
SRT	T-48740	Renal Vein
SRT	T-46659	Segmental Artery
SRT	T-4668A	Arcuate Artery of the Kidney
SRT	T-4667D	Interlobar Artery of Kidney
MRUS	V12115-01	Main Renal Artery

C.18. CID (12116) Vessel Segment Modifiers

CSD	CV	Code Meaning
SRT	G-A119	Distal
SRT	G-A188	Mid-longitudinal
SRT	G-036A	Origin of vessel
SRT	G-A118	Proximal
SRT	R-1025B	Dilated portion of segment

C.19. Mapping between Modality measurements and DICOM Concepts.

C.19.1. Vascular Measurements

MODALITY Label	*DICOM Mapping*
<Vasculature Anatomic Location> ED	11653-3, LN, End Diastolic Velocity
<Vasculature Anatomic Location> MD	11665-7 , LN, Minimum Diastolic Velocity
<Vasculature Anatomic Location> PS	11726-7, LN, Peak Systolic Velocity
<Vasculature Anatomic Location> TAMEAN	20352-1, LN, Time averaged mean velocity
<Vasculature Anatomic Location> TAMAX	11692-1, LN, Time averaged peak velocity
<Vasculature Anatomic Location> PV	11726-7, LN, Peak Velocity
<Vasculature Anatomic Location> PI	12008-9, LN, Pulsatility Index
<Vasculature Anatomic Location> RI	12023-8, LN, Resistivity Index
<Vasculature Anatomic Location> S/D	12144-2, LN, Systolic to Diastolic Velocity Ratio
<Vasculature Anatomic Location> D/S	M12119-04, MRUS, Diastolic to SystolicVelocity Ratio
<Vasculature Anatomic Location> AT	20168-1, LN, Acceleration Time
<Vasculature Anatomic Location> DT	20217-6, LN, Deceleration Time
<Vasculature Anatomic Location> PPG	20247-3, LN, Peak Gradient
<Vasculature Anatomic Location> MPG	20256-4, LN, Mean Gradient
<Vasculature Anatomic Location> MMPG	M12119-01, MRUS, Mean Velocity Mean Pressure Gradient
<Vasculature Anatomic Location> VTI	M12119-02, MRUS,Velocity-Time Integral
<Vasculature Anatomic Location> HR	8867-4, LN, Heart Rate
<Vasculature Anatomic Location>	M12119-03, MRUS, Angle
<Vasculature Anatomic Location> VD	R-1025C, SRT, Vessel Intimal Diameter
<Vasculature Anatomic Location> VolFlow	M12119-06, MRUS, Vol Flow(TAMAX)
<Vasculature Anatomic Location> VolFlow.TAMEAN	M12119-07, MRUS,Vol Flow(TAMEAN)

C.19.2. Extracranial Arteries

MODALITY Label	*DICOM Mapping*
Bulb	T-45170,SRT,Carotid Bulb
CCA	T-45100,SRT,Common Carotid Artery
ECA	T-45200,SRT,External Carotid Artery
ICA	T-45300,SRT,Internal Carotid Artery
Subclav A	T-46100,SRT,Subclavian Artery
Vert A	T-45700,SRT,Vertebral Artery

C.19.3. Upper Extremity Arteries

MODALITY Label	*DICOM Mapping*
Axill A	T-47100,SRT,Axillary Artery
Brachial	T-47160, SRT, Brachial Artery
Radial A	T-47300,SRT,Radial Artery
Subclav	T-46100, SRT, Subclavian Artery
Ulnar A	T-47200,SRT ,Ulnar Artery

C.19.4. Upper Extremity Arteries(unilateral)

MODALITY Label	*DICOM Mapping*
Innom A	T-46010, SRT, Innominate Artery

C.19.5. Upper Extremity Veins

MODALITY Label	*DICOM Mapping*
Axill V	T-49110,SRT ,Axillary vein
Basilic V	T-48052,SRT,Basilic vein
Brachial V	T-49350,SRT,Brachial vein
Cephalic V	T-49240,SRT,Cephalic vein
Radial V	T-49340,SRT,Radial vein
Subclav V	T-48330,SRT,Subclavian vein
Ulnar V	T-49330,SRT,Ulnar vein

C.19.6. Lower Extremity Arteries

MODALITY Label	*DICOM Mapping*
C.Iliac A	T-46710,SRT,Common Iliac Artery
A.Tib A	T-47700,SRT ,Anterior Tibial Artery
CFA	T-47400,SRT ,Common Femoral Artery
Dors.Ped A	T-47741,SRT,Dorsalis Pedis Artery
Ex.Iliac A	T-46910,SRT ,External Iliac Artery
IIA	T-46740,SRT ,Internal Iliac Artery
Peroneal A	T-47630,SRT ,Peroneal Artery
Pop A	T-47500,SRT ,Popliteal Artery
P.Tib A	T-47600,SRT ,Posterior Tibial Artery
PFA	T-47440,SRT ,Profunda Femoris Artery

SFA	T-47403 ,SRT ,Superficial Femoral Artery
TP Trunk A	V12109-01,MRUS,TP Trunk Artery

C.19.7. Lower Extremity Veins

MODALITY Label	*DICOM Mapping*
A.Tib V	T-49630,SRT,Anterior Tibial Vein
CFV	G-035B,SRT,Common Femoral Vein
C.Iliac V	T-48920,SRT,Common Iliac Vein
Ex.Iliac V	T-48930,SRT,External Iliac Vein
Sural V	T-4942D,SRT,Gastrocnemius vein
Saph V	T-49530,SRT,Great Saphenous Vein
SSV	T-49550,SRT,Lesser Saphenous Vein
Peroneal V	T-49650,SRT,Peroneal Vein
Pop V	T-49640,SRT,Popliteal Vein
P.Tib V	T-49620,SRT,Posterior Tibial Vein
PFV	T-49660,SRT,Profunda Femoris Vein
Soleal V	G-036B,SRT,Soleal vein
SFV	G-035A,SRT,Superficial Femoral Vein

Right Hepatic V	T-48725,SRT,Right Hepatic Vein
M Hepatic V	T-48726,SRT,Middle Hepatic Vein
Portal V	T-48810,SRT,Portal Vein
IVC	T-48710,SRT,Inferior Vena Cava
Splenic V	T-48890,SRT,Splenic Vein
SMV	T-48840,SRT,Superior Mesenteric Vein