

Mobile Viewer

Operator's Manual

WARNING

- Federal Law (USA) restricts this device to sale by or on the order of a physician or other practitioner licensed by U.S. state law to use or order the use of this device.
-
-

Intellectual Property Statement

SHENZHEN MINDRAY BIO-MEDICAL ELECTRONICS CO., LTD. (hereinafter called Mindray) owns the intellectual property rights to this Mindray product and this manual. This manual may refer to information protected by copyrights or patents and does not convey any license under the patent rights of Mindray, nor the rights of others.

Mindray intends to maintain the contents of this manual as confidential information. Disclosure of the information in this manual in any manner whatsoever without the written permission of Mindray is strictly forbidden.

Release, amendment, reproduction, distribution, rental, adaption and translation of this manual in any manner whatsoever without the written permission of Mindray is strictly forbidden.



mindray, **MINDRAY**, and **MINDRAY** are the registered trademarks or trademarks owned by Mindray in China and other countries. All other trademarks that appear in this manual are used only for editorial purposes without the intention of improperly using them. They are the property of their respective owners.

This posting serves as notice under 35 U.S.C.§287(a) for Mindray patents: <http://www.mindrayna.com/patents>.

Manufacturer's Responsibility

Contents of this manual are subject to changes without prior notice.

All information contained in this manual is believed to be correct. Mindray shall not be liable for errors contained herein nor for incidental or consequential damages in connection with the furnishing, performance, or use of this manual.

Mindray is responsible for the effects on safety, reliability and performance of this product, only if the product is used in accordance with the instructions for use.

Company Contact

Manufacturer: Shenzhen Mindray Bio-Medical Electronics Co., Ltd.
Address: Mindray Building, Keji 12th Road South, High-tech Industrial park, Nanshan, Shenzhen 518057, P.R.China
Website: www.mindray.com
E-mail Address: service@mindray.com.cn
Tel: +86 755 81888998
Fax: +86 755 26582680

Distributor: Mindray DS USA, Inc.
Address: 800 MacArthur Boulevard, Mahwah, New Jersey, 07430 USA
Tel: 1.800.288.2121, 1.201.995.8000
Website: www.mindray.com

Preface

Manual Purpose

This manual contains the instructions necessary to operate the product safely and in accordance with its

This page intentionally left blank.

Contents

1 Safety	1 - 1
1.1 Safety Information	1 - 1
1.1.1 Warnings	1 - 1
1.1.2 Cautions	1 - 1
2 Overview	2 - 1
2.1 Overview	2 - 1
2.2 Installation Requirements	2 - 1
2.2.1 For Android Client	2 - 1
2.2.2 For iOS Client	2 - 1
2.3 Installing the Mobile Viewer	2 - 2
2.3.1 For Android Client	2 - 2
2.3.2 For iOS Client	2 - 2
2.4 Starting the Mobile Viewer	2 - 2
3 Basic Operations	3 - 1
3.1 Settings	3 - 1
3.1.1 Setting Server	3 - 1
3.1.2 Setting Monitor Data	3 - 2
3.2 Login	3 - 2
3.3 Log-Out	3 - 2
3.4 Patient Selection Mode	3 - 2
3.4.1 Selecting a Department	3 - 2
3.4.2 Patient Selection in Manual Mode	3 - 3
3.4.3 Patient Selection in Care Group Mode	3 - 6
3.5 Monitoring Multiple Patients	3 - 7
3.5.1 Viewing Parameters	3 - 7
3.5.2 Viewing Alarm Messages	3 - 8
3.6 Monitoring a Single Patient	3 - 10
3.6.1 View Bed	3 - 11
3.6.2 Event Review	3 - 12
4 Troubleshooting	4 - 1
4.1 Failed to Log on to Mobile Viewer	4 - 1
4.2 The List of My Patients Is Blank after Logging to Mobile Viewer	4 - 1

This page intentionally left blank.

1 Safety

1.1 Safety Information

WARNING

- Indicates a potential hazard or unsafe practice that, if not avoided, could result in death or serious injury.
-
-

CAUTION

- Indicates a potential hazard or unsafe practice that, if not avoided, could result in minor personal injury or product/property damage.
-

NOTE

- Provides application tips or other useful information to ensure that you get the most from your product.
-

1.1.1 Warnings

WARNING

- The user of the equipment should receive sufficient training. Anyone unauthorized or untrained must not perform any operation on it.
 - To avoid inadvertent disconnection, route all cables in a way to prevent a stumbling hazard. Wrap and secure excess cabling to avoid risk of entanglement or strangulation by patients or personnel.
 - When disposing of the package material, observe applicable local or hospital's waste control regulations and keep it out of children's reach.
 - Before connecting the equipment to the power line, check that the voltage and frequency ratings of
-

This page intentionally left blank.

2 Overview

2.1 Overview

The Mobile Viewer is a mobile application independent of the Central Monitoring System, supporting Android and iOS systems. Doctors, nurses and other medical personnel can use Mobile Viewer to view the data from patient monitors, telemetry devices, and other monitoring devices admitted by the BeneVision Central Monitoring System (hereinafter referred to as the CMS).

The Mobile Viewer installation for Android and iOS clients are the same, only installation screenshots for Android client are taken for reference in this manual.

The Mobile Server provides monitoring data to the Mobile Viewer and acts as an interface to the BeneVision CMS. For details on the Mobile Server, see Mobile Server Installation Guide (P/N: 046-011066-00).

WARNING

- **The Mobile Viewer is not intended for real-time or primary monitoring. It cannot be used as a device for issuing alarms. There is no audible alarm sound in the Mobile Viewer, and all the data is delayed. Always refer to your primary monitoring source for current information, real-time patient data and combine this data with personal clinical observation of the patient before administering interventions.**
-
-

2.2 Installation Requirements

2.2.1 For Android Client

The installation requirements for Android client are shown as below.

Item	Requirement
Platform	Cell phone whose operating system is Android 4.4 or above
CPU	1.3GHz or above, quad core or above
RAM	1.5GB or above
Screen resolution	1920×1080 recommended

Table 2-1 Requirements for Android Client

2.2.2 For iOS Client

The installation requirements for iOS client are shown as below.

Item	Requirement
Platform	Cell phone whose operating system is iOS 9.2 or above
iPhone	iPhone 6, iPhone 6 Plus or above
iPad	iPad mini2 or above

Table 2-2 Requirements for iOS Client

2.3 Installing the Mobile Viewer

2.3.1 For Android Client

To install the Mobile Viewer, follow this procedure:


1. From the Google Play Store, search for **Mindray Mobile Viewer**.
2. Select **INSTALL**.

2.3.2 For iOS Client

To install the Mobile Viewer, follow this procedure:

1. From the Apple AppStore, search for **Mindray Mobile Viewer**.
2. Select **INSTALL**.

2.4 Starting the Mobile Viewer

Select the Mobile Viewer icon  to start the application, as shown in Figure 2-1.

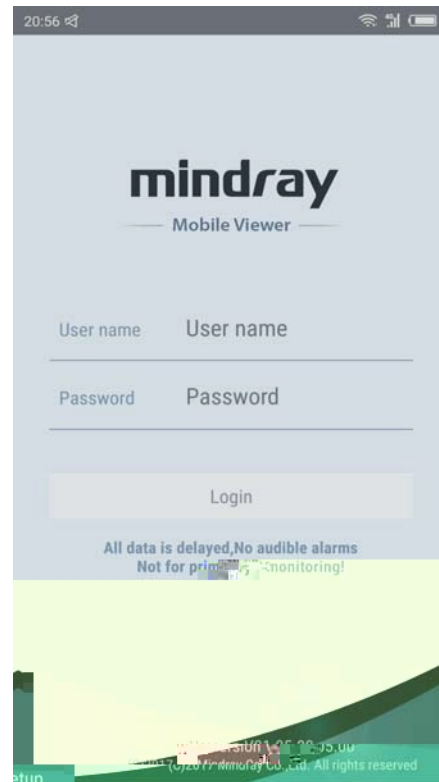


Figure 2-1 Example Mobile Viewer Login Screen

NOTE

- Before using Mobile Viewer for the first time, first configure this application by following steps in Section

3 Basic Operations

3.1 Settings

1. Select **Setup** on the login screen to enter the **Setup** screen.

Figure 3-1 Example Setup Screen

2. Set the required items.
-

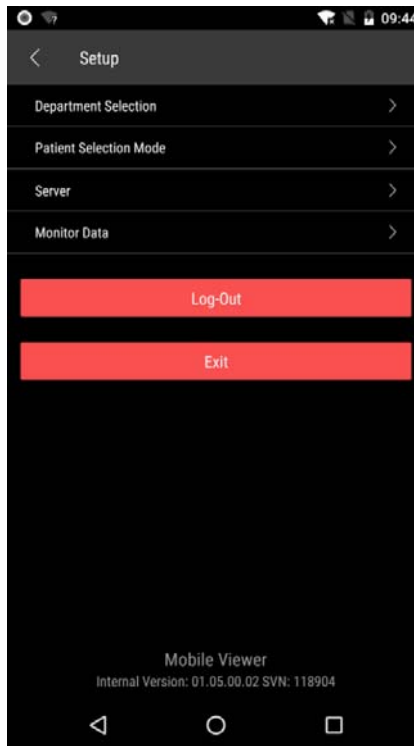


Figure 3-4 Example Mobile Viewer Setup Screen

2. Select **Department Selection**. The **Department Selection** screen is displayed as shown below.




Figure 3-5 Example Department Selection Screen

3. Select or unselect the checkbox to follow or unfollow a department.

3.4.2 Patient Selection in Manual Mode

3.4.2.1 Setting Patient Selection Mode to Manual

To set **Patient Selection Mode** to **Manual**, follow this procedure:

1. Click the  button on the **My Patients** screen. The **Setup** screen is displayed.
2. Select **Patient Selection Mode**.

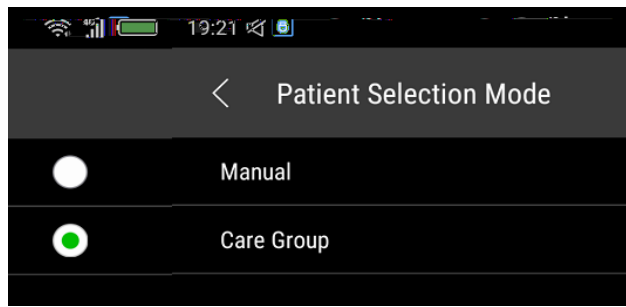


Figure 3-6 Example Patient Selection Mode Screen

3. Select **Manual**.

3.4.2.2 Following/Unfollowing Patients

Because no patients have been selected at the first time of login, the **My Patients** screen is blank.





Figure 3-7 Example My Patients Screen

1. Select the  icon on the toolbar of **My Patients** screen to enter the **Patients Management** screen. All the patients which are authorized to view are displayed by grouping of departments.
2. Select or unselect the checkbox on the right of a patient to follow/unfollow this patient. A maximum of 32 patients can be followed; select anywhere on the left of the check box of a patient to view the real-time monitoring parameter and waveform of this patient. For details, see **3.6 Monitoring a Single Patient**.

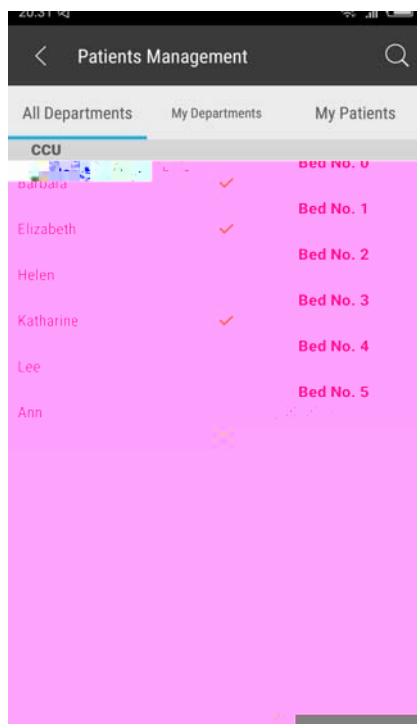


Figure 3-8 Example Patients Management Screen

- Sliding the **All Departments** tab to left goes to the **My Departments** tab. This tab displays the list of patients under the departments selected on the **Department Selection** screen.

Select or unselect the checkbox on the right of a patient to follow/unfollow this patient. A maximum of 32 patients can be followed; select anywhere on the left of the check box of a patient to view the real-time monitoring parameter and waveform of this patient. For details, see **3.6 Monitoring a Single Patient**.

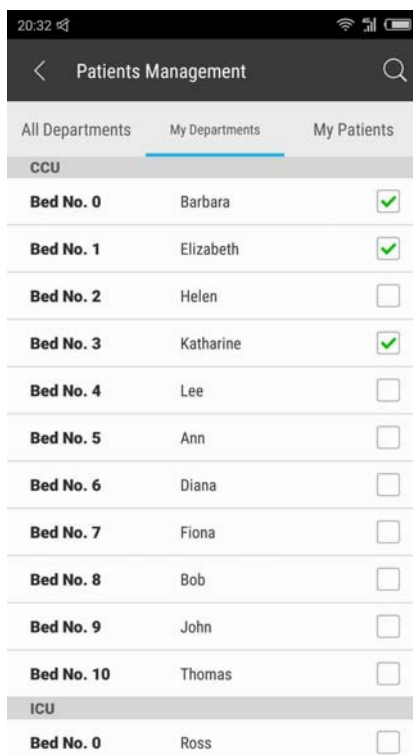




Figure 3-9 Example My Departments Tab

NOTE

- If you have not selected a department on the Department Selection screen, the My Departments tab is blank.
4. Sliding the My Departments tab to left goes to the My Patients tab. This tab displays the list of currently followed patients. Slide leftward on a patient to display . You can select  to unfollow this patient.

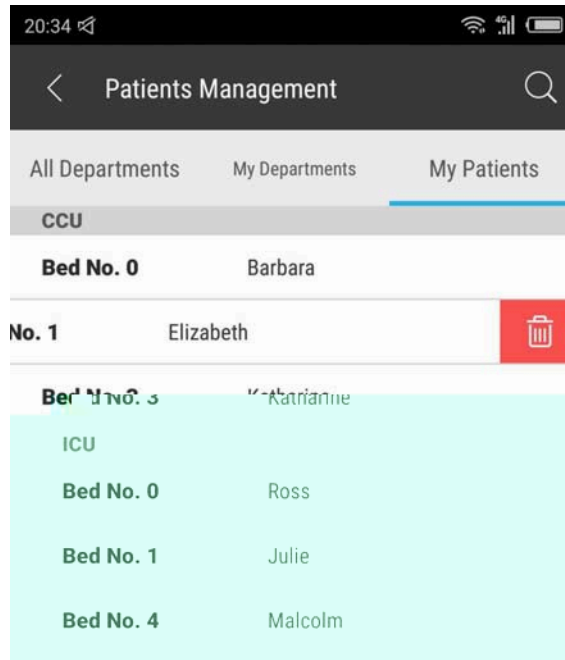




Figure 3-10 Example My Patients Screen

3.4.2.3 Searching Patients

To search patients, follow this procedure:

1. Select the  icon on the toolbar of Patients Management to enter the patient-searching screen.
2. Enter the patient's name, bed number or room number in the search box, and select **Search**. The search result will be displayed below. You can perform following/unfollowing operation in the search result, or select the  icon in the search box to clear the entered content in the search box.

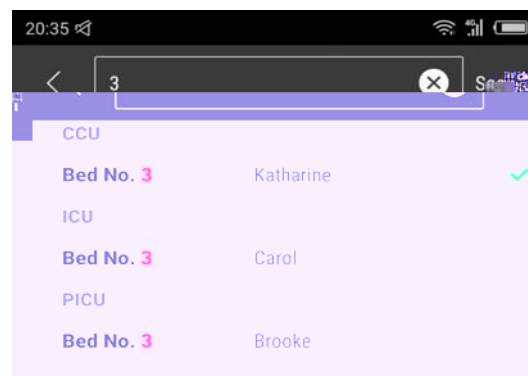



Figure 3-11 Example Patients Searching Screen

3.4.3 Patient Selection in Care Group Mode

To set Patient Selection Mode to Care Group, follow this procedure:

1. Click the  button on the My Patients screen. The Setup screen is displayed.
2. Set Patient Selection Mode to Care Group.
Care groups are displayed in the form of "department+shift".

3. Select or unselect the checkbox on the right side of a care group to follow or unfollow a care group, as shown below.

Figure 3-12 Example Care Group Selection Screen

When you return to **My Patients** screen, the patients selected for care groups are displayed. Besides, the icon is not displayed in the tool bar of **My Patients** screen.

NOTE

- The care group list only displays care groups for departments selected in the **Department Selection** tab and the selected care groups. Therefore, before selecting a care group, select a department in the **Department Selection** tab. Otherwise, no care group is displayed.
 - When care groups are configured via the CMS, check that the departments where care groups are located are configured. Otherwise, the configured care group cannot be displayed at the **Mobile Viewer**.
 - If you have unselected a department in the **Department Selection** tab, care groups for this department are unfollowed simultaneously.
 - Patient Selection Mode cannot be set to Care Group in Demo mode.
-

3.5 Monitoring Multiple Patients

3.5.1 Viewing Parameters

Choose either of the following ways to view parameters and alarm messages of followed patients,

Select the patients that need to be followed in the **All Patients** tab or **My Departments** tab on the patient management screen,

After selecting the care groups that need to be followed on the **Patient Selection Mode** screen, return to **My Patients** home screen.

In the area of each patient, the patient's personal information (the bed No., name, etc.) is displayed on the upper left side, and the alarm message of this patient is on the right; the parameter area is at the lower part. You can drag leftward and rightward in the pa



Figure 3-13 Example Multiple Patients Monitoring Screen

3.5.2 Viewing Alarm Messages

The latest alarm message is displayed in the upper right corner of each patient's area. Select the alarm message to display the alarm message box and show more alarm messages. If there is "✓" before a message, this alarm has been acknowledged; if time is displayed on the right of the message, the time is the time when the alarm is triggered.

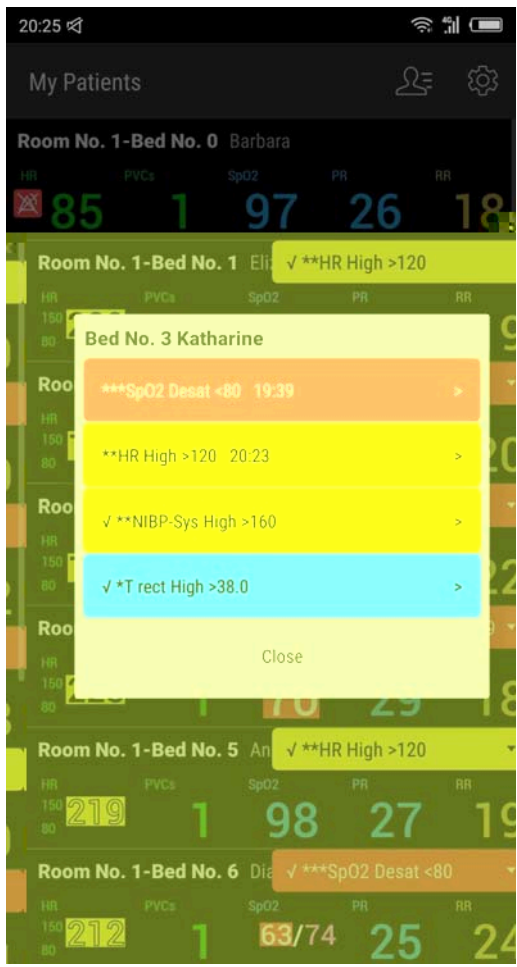


Figure 3-14 Example Screen of Viewing Alarm Messages

You can select an alarm message to view alarm details (details not provided for technical alarms). You can drag leftward and rightward in the parameter area and waveform area to view more details.

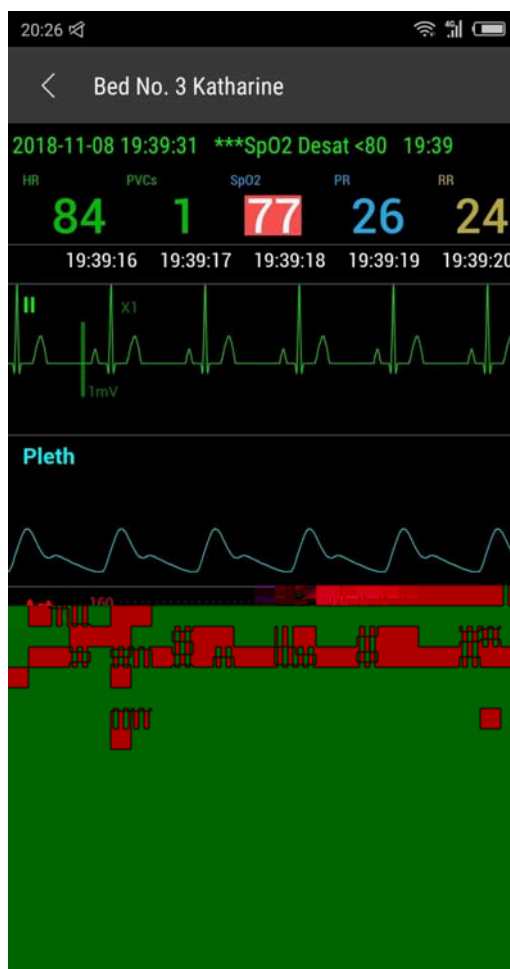


Figure 3-15 Example Alarm Details

3.6 Monitoring a Single Patient

Select a patient on the **My Patients**, **All Departments**, or **My Departments** screen to access the monitoring screen of this patient. This screen consists of the **View Bed** and **Event Review** tabs.



Figure 3-16 Example Single Patient Screen


3.6.1 View Bed

The View Bed screen contains the alarm area, parameter area, and waveform area from top down.

Alarm area: It displays the latest alarm message. You can select to view more alarms and alarm details.

Parameter area: It displays the real-time parameters. You can drag leftward and rightward to view more parameters. If a parameter has a background color and blinks, this parameter is in the alarm status currently. If the parameter is in the hollow style, this parameter is unreliable.

Waveform area

For Android cell phones: It displays the real-time waveform. Select  to freeze the waveform and change the waveform background to gray. You can drag the waveform leftward to view earlier waveforms. Select this button again to cancel the freezing operation.


For iPhones: The  icon is not displayed. You can free waveforms either by double clicking real-time waveforms or touching and holding the real-time waveform area. If you wish to unfreeze waveforms, double click or touch and hold the frozen waveform area.



Figure 3-17 Example View Bed Screen

3.6.2 Event Review

Events of this patient can be reviewed on this screen. When **Event Level** is selected for the first time, events will be sorted in the descending order of priority; if it is selected again, events will be sorted in the ascending order of priority. When **Event Time** is selected for the first time, events will be sorted in the descending order of time; if it is selected again, events will be sorted in the ascending order of time.

Select an event to view details of this event. It is the same as the operation of viewing alarm details.

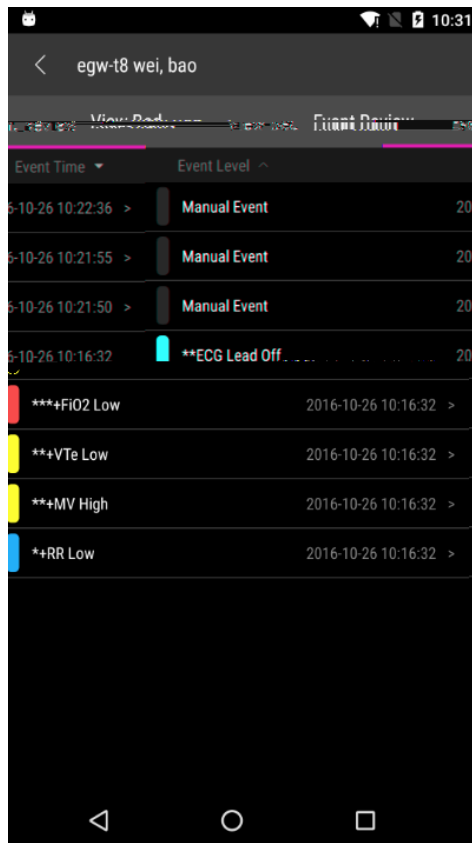


Figure 3-18 Example Event Review Screen

This page intentionally left blank.

4 Troubleshooting

4.1 Failed to Log on to Mobile Viewer

Please try the following operations:

Check whether the server IP address and port number in Mobile Viewer settings are configured correctly. If the configuration is correct, try to open `http://Server:port/index.html` (Server is the IP address or domain name of the server, and port is the port number of the server) in the mobile phone browser.

If "It works!" is displayed, the network is normal; otherwise check whether the cellular data or Wi-Fi connection is normal or whether the corresponding port is opened for the firewall of Mobile Server. If the network connection is normal, check whether the user name or password is correct.

If encrypted communication is adopted and login failure is prompted, clear the data and cache of this application from system settings or uninstall and reinstall this application, and try it again.

If multiple users use the same account, contact your administrator to check if the local account or domain account of the server is locked. Accounts are locked when other users made several attempts to log in using a wrong password. If this is the cause of the problem, we suggest that the administrator creates accounts for every user or change the account-lock security policy.

4.2 The List of My Patients Is Blank after Logging to Mobile Viewer

Please try the following operations:

Follow patients or care groups. For how to follow them, see *3.4.2.2 Following/Unfollowing Patients* and *3.4.3 Patient Selection in Care Group Mode*.

If the patient selection mode is care group, ensure that the shift of care groups is correct.

This page intentionally left blank.



046-011215-00(5.0)